



Veterinary Color Doppler Ultrasound System

User Manual

Statement

Thank you for selecting Veterinary Color Doppler Ultrasound System.

Prior to using the system, please read this user manual carefully.

In addition, keep this user manual so that you may read it at any time when necessary.

Product Information

Product Name: Veterinary Color Doppler Ultrasound System

Product Model: VU40

The system consists of the console (including display and control panel), software package (software name: Color Doppler Ultrasound System Software, release version: V1), and probes.

Optional accessories: lithium battery, printer, foot switch, gel warmer, ECG (a standard feature for VU60).

Optional ultrasound probes: 3C5PD, 7L4PD, 5P1PA, 6C1PD, 10L2PD, 3P2PA

Application range: The system is intended for veterinary use in clinical ultrasound examination and diagnosis.

Register/manufacturer: Wuhan Zoncare Bio-medical Electronics Co., Ltd

Address: #380, High-tech 2nd road, Eastlake high-tech district, Wuhan, Hubei, P. R. China

Address of manufacturing: #380, High-tech 2nd road, Eastlake high-tech district, Wuhan, Hubei, P. R. China

Production date: see tag

Service life: 10 years

Intellectual Property Statement

Wuhan Zoncare Bio-medical Electronics co., Ltd owns the intellectual property rights to this product and this manual. (Hereinafter referred to as “Zoncare”)

No part of this manual may be reproduced, transferred, or copied, in any form or by any means, without written permission by Zoncare.

ZONCARE is the registered trademark or trademark of Zoncare.

Responsibility of the Manufacturer

Zoncare is responsible for the effects on safety, reliability, and performance of the product, only if:

- All installation operations, expansions, adjustments, upgrades and repairs of this product are conducted by Zoncare authorized personnel;
- All components for replacement, accessories and consumables are original of Zoncare or approved by Zoncare;
- Electrical installation complies with the applicable national standards and the requirements of this user manual;
- Use this product only in accordance with this user’s manual.

About this Manual

Issue date: 2024-07

Version: 3.0

This manual details all information necessary for safe operation of the system. The applications, functions, operations and maintenance of the product are described with the most comprehensive configuration in this manual. If there is any discrepancy between the description in the manual and the physical one, please prevail in kind. If you have questions, please contact us.

Figures showed in this manual may be different from physical one, please prevail in kind.

This manual is intended for users familiar with the basic principles and techniques of ultrasound. It does not involve ultrasound training or medical procedures.

Conventions Used in this Manual

Before using the system, read carefully and be sure to completely understand these conventions in this manual.

Symbols and conventions	Description
DANGER	DANGER indicates a hazardous situation which, if not avoided, will result in death or serious injury.
 Warning	WARNING indicates a potentially hazardous situation, which, if not avoided, may result in physical injury or death.
CAUTION	CAUTION Indicates a potentially hazardous situation, which, if not avoided, could result in minor or moderate injury or equipment damage.
	Patient /user infection due to contaminated equipment.
NOTE	Provide additional Information.
Click	Press the [Set] button or tap the menu item on the Touch Screen.
Double-click	Press the [Set] button twice in quick succession.
Select	Highlight a menu item with the trackball.
[Bold]	Physical buttons or knobs on the device, prompts or menu items on the touch screen.
<Keyboard>	Keyboard keys.

Warranty

The warranty period is subject to the sale contract.

Consumables refer to disposable consumables that need to be replaced after each use or vulnerable materials that need to be replaced regularly. Consumables are not covered by warranty.

The warranty period starts from the “installation date” filled in the “Product Warranty Card” that accompanies the product. The “Product Warranty Card” is the only voucher for calculating the warranty period and enjoying the warranty service.

To protect your rights and interests, please fill in the warranty card after the system is installed, and give it to the installer or mail it to the Customer Service Department of Zoncare Company.

During the warranty period, Zoncare will provide you with free warranty service; beyond the warranty period, Zoncare will provide maintenance service for products under the condition of reasonable labor fee, spare parts fee and transportation fee.

But please note that even during the warranty period, the following condition is not covered by the free warranty. Zoncare will charge for repair and accessories:

- Artificial damage;
- Improper use;
- The voltage of the power grid is beyond the scope specified by the product;
- Irresistible natural disasters;
- Replace or use of parts, accessories, and consumables not approved by Zoncare or maintain the system by unauthorized personnel;
- Failures not arise from the product itself;
- Failure to follow any operation instruction of the user manual.

Disclaimer

Zoncare does not assume any responsibility for unintended use, mis-operation by unqualified medical personnel or failure to follow operation instruction of the user manual.

Zoncare does not assume any responsibility for any medical disputes arising from the rental of equipment to third parties or other institutions.

Contents

Chapter 1	Safety	1
1.1	Safety Information	1
1.1.1	Precautions.....	1
1.1.2	Labels and Symbols.....	5
1.2	Application of Acoustic Power	8
1.2.1	ALARA.....	8
1.2.2	Bioeffect.....	8
1.2.3	Output Display.....	9
1.2.4	Probe Surface Temperature	9
1.2.5	Acoustic Power Control.....	9
Chapter 2	System Overview	11
2.1	Application Range	11
2.2	Contraindications	11
2.3	System Configuration	11
2.3.1	Standard Configuration	11
2.3.2	Optional Probes.....	11
2.3.3	Optional Accessories.....	11
2.4	System Components	13
2.4.1	Console	13
2.4.2	Control Panel.....	15
2.4.3	Trackball	18
2.4.4	Keyboard	18
2.4.5	Front Panel.....	20
2.4.6	I/O Board	21
2.4.7	Power Supply Panel.....	22
Chapter 3	Preparing the System	23
3.1	Moving the system.....	23
3.1.1	Transporting	23
3.1.2	Moving	23
3.2	Positioning	24

3.3	Connecting the System	24
3.3.1	External Power Supply	25
3.3.2	Battery Power Supply	25
3.4	Power On/ Off the System	26
3.4.1	Power on	26
3.4.2	Power off	27
3.4.3	Standby	27
3.5	Mechanical Adjustment	28
3.5.1	Adjust the Monitor	28
3.5.2	Adjust the Control Panel	30
3.5.3	Adjust the Touch Screen	30
3.6	Connect / Remove the Probe	31
3.6.1	Connect the Probe	31
3.6.2	Remove the Probe	31
3.7	Install the Gel Warmer	32
3.8	Foot Switch	33
3.9	Connect the Network	33
3.10	Connect Peripheral Device	33
3.10.1	Connect USB Device	33
3.10.2	Connect Printer	34
3.11	ECG	35
3.11.1	ECG Operation	35
3.11.2	ECG Maintenance	36
3.12	Screen	36
3.12.1	Home Screen	36
3.12.2	Touch Screen	37
Chapter 4	System Settings	39
4.1	Overview	39
4.2	System Preset	39
4.2.1	Region	39
4.2.2	General	41
4.2.3	Image	42
4.2.4	Application	43
4.2.5	Customize	45

4.2.6	Admin	45
4.3	Exam Preset	48
4.3.1	Add Exam Mode.....	49
4.3.2	Remove Exam Mode.....	49
4.3.3	Create/Delete User-defined Exam Mode.....	50
4.3.4	Adjust Exam Mode Display Position	50
4.4	Measure Preset	50
4.4.1	General Measurement Preset.....	50
4.4.2	Application Measurement Preset	51
4.4.3	Report Template	54
4.5	zWorkflow Preset.....	55
4.5.1	Workflow Protocol	55
4.5.2	New Protocol	56
4.5.3	Basic zWorkflow Procedures	56
4.5.4	Section Operation.....	57
4.6	Network Preset	57
4.7	Print Preset	58
4.8	Maintenance Preset.....	59
4.8.1	System Information	60
4.8.2	Detailed Information	60
4.8.3	Option	60
4.8.4	Other.....	60
Chapter 5	Preparing an Exam	62
5.1	Animal Information.....	62
5.1.1	New Animal.....	62
5.1.2	Retrieve Animal Information (Station)	65
5.1.3	Retrieve Animal Information (DICOM)	66
5.2	Select Probe and Exam Mode.....	66
5.3	Select Imaging Mode.....	67
5.4	Resume/Activate Exam	67
5.4.1	Resume Exam.....	67
5.4.2	Activate Exam	68
5.5	Cancel / End Exam.....	68
5.5.1	Cancel Exam	68

5.5.2	End Exam.....	68
Chapter 6	Optimizing the Image.....	69
6.1	Imaging Mode.....	69
6.2	Operation Interface.....	69
6.3	B-mode	69
6.3.1	Basic Procedure of B-mode	69
6.3.2	Image Optimization (B)	70
6.4	M-mode.....	75
6.4.1	Basic Procedure of M-mode.....	75
6.4.2	Image Optimization (M).....	76
6.5	Color Mode	77
6.5.1	Basic Procedure of Color Mode	77
6.5.2	Basic Procedure of PDI mode.....	78
6.5.3	Image Optimization (Color/PDI)	79
6.6	Doppler Imaging Mode	83
6.6.1	Basic Procedure of PW-mode.....	83
6.6.2	Basic Procedure of CW mode.....	84
6.6.3	Image Optimization (PW/CW).....	86
6.7	Anatomical M-mode.....	90
6.7.1	Linear Anatomical M-mode	90
6.7.2	Curved Anatomical M-mode.....	90
6.8	Color M-mode.....	91
6.9	Tissue Doppler Imaging (TDI)	92
6.9.1	TDI-modes.....	92
6.9.2	Basic Procedure of TDI mode	92
6.10	Panoramic Imaging.....	93
6.10.1	Basic Procedure of Panoramic Imaging.....	93
6.10.2	Image Optimization (Pano)	94
6.10.3	Image Quality	94
6.11	Elastography.....	95
6.11.1	Basic Procedure of Elastography.....	95
6.11.2	Image Optimization (Elastography).....	96
Chapter 7	Image Review and Management.....	97

7.1	Splitting Display	97
7.2	Image Magnification	98
7.2.1	Global Zoom.....	98
7.2.2	Local Zoom.....	98
7.2.3	Fullscreen	99
7.3	Freeze the Image	99
7.4	Cine Replay	99
7.4.1	Cine Replay Region	100
7.4.2	Manual Replay	101
7.4.3	Auto Replay	101
7.5	Annotation.....	101
7.5.1	Comment.....	101
7.5.2	Arrow	103
7.5.3	Body Mark	103
Chapter 8	Image Measurement	105
8.1	Basic Operating Procedure	105
8.2	General Measurement.....	106
8.2.1	2D General Measurement.....	106
8.2.2	M General Measurement	112
8.2.3	Doppler General Measurement.....	114
8.3	Application Measurement.....	119
8.3.1	Abdomen	119
8.3.2	Reproduction	122
8.3.3	Cardiology	123
8.3.4	Small Parts	152
8.3.5	Vascular	153
Chapter 9	Report	159
9.1	View the Report	159
9.2	Edit the Report.....	160
9.2.1	Comment.....	160
9.2.2	Add Image	160
9.3	Review the Report.....	161
9.4	Print the Report.....	161

9.5	Back up the Report.....	161
9.5.1	Save	161
9.5.2	Load.....	161
9.5.3	Export	161
Chapter 10 Animal Data Management		163
10.1	Storage	163
10.1.1	Image Storage.....	163
10.1.2	Cine Storage	163
10.2	Image Viewing	164
10.2.1	Current Animal.....	164
10.2.2	Previous Animals.....	165
10.3	Delete Image/Data.....	166
10.3.1	Current Animal.....	166
10.3.2	Previous Animals.....	166
10.4	Image/Data Recovery.....	167
10.5	Exporting Image/Data.....	167
10.5.1	Exporting to USB Storage Device.....	168
10.5.2	Exporting to DVD Disc (Optional)	168
10.5.3	Exporting to DICOM Server	169
10.6	Disk Space Detection	169
10.7	Task Manager	169
10.8	Image Demo	169
Chapter 11 DICOM.....		171
11.1	DICOM Preset	171
11.1.1	DICOM Local Preset	171
11.1.2	Service Preset.....	172
11.2	DICOM Service.....	181
11.2.1	DICOM Storage.....	181
11.2.2	DICOM Print.....	182
11.2.3	DICOM Worklist.....	182
11.2.4	DICOM MPPS	183
11.2.5	DICOM Storage Commitment	184
11.2.6	DICOM Query / Retrieve	184

11.3	Structured Report	185
Chapter 12	Probe and Biopsy	187
12.1	Probe	187
12.1.1	Structure of Probe	187
12.1.2	Probe Usage	187
12.1.3	Probe Cleaning.....	188
12.1.4	Probe Disinfection	189
12.1.5	Probe Maintenance	190
12.2	Biopsy	191
12.2.1	Calibrate the Biopsy Guide Line.....	191
12.2.2	Biopsy Procedure	192
12.2.3	Bracket Cleaning and Disinfection	193
12.2.4	Bracket Storage and Transportation	194
Chapter 13	System Maintenance	195
13.1	External Cleaning	195
13.1.1	Clean the Trackball.....	195
13.1.2	Clean the Probe Holder.....	196
13.1.3	Clean the Gel Warmer.....	197
13.1.4	Clean the Printer	197
13.1.5	Clean the ECG equipment	198
13.2	Safety Check	198
13.3	Troubleshooting	199
13.4	Disposal	199
13.5	After Sales Service	200
Appendix A	Technical Specifications	201
Appendix B	EMC Statement	202
Appendix C	Toxic and Hazardous Substances or Elements.....	210

Chapter 1 Safety

1.1 Safety Information

Read, understand and strictly follow the instructions before using the system to ensure the safety of animal and operator.

This system should be used by a professional clinician or under the guidance of a professional clinician. Unauthorized person or untrained person shall not perform any operation.

Manufacturer is responsible for the effects on safety, reliability, and performance of the product, only if following precautions are strictly followed.

1.1.1 Precautions

1.1.1.1 System safety

DANGER

- **DO NOT** operate the system in the presence of flammable gases or anesthetics or ethyl alcohol. Explosion may result.
 - If flammable substances are detected, **DO NOT** plug in the power cord or power on the system.
 - If flammable substances are detected after the system is powered on, **DO NOT** attempt to shut down the system or unplug the power cord.
 - If flammable substances are detected, exhaust the air in the area and make well ventilation before shutting down the system.
- **Never** operate the system in thunderstorm weather.
- **DO NOT** connect the grounding wire to any gas pipeline or water pipe. Otherwise it may lead to poor grounding or explosion risk.
- **Connect** the grounding wire correctly before powering on the system. Make sure the system grounding is always well-connected to the earth when operating the system.
- **Ensure** that a standard three-pronged grounding plug is used. Push the power plug securely to the hospital grade grounding outlet of appropriate power rating.
- **Never** use an adapter.
- **DO NOT** place liquids on or above the console. Spilled liquid may contact live parts and increase the risk of electric shock. If liquid is accidentally into the system, stop using the system immediately and shut down the system, contact Zoncare Customer Service Department or sales representative.
- **To avoid** the risk of electric shock, the device must be connected a power supply with protective grounding.
- **Never** allow the animal to contact the live part of the system or



other device, e.g. Signal I/O ports. Electric shock may result.

- **DO NOT** use the system with high-frequency surgical equipment, high frequency electrotome, or defibrillator.
- Unauthorized personnel are **NOT** allowed to remove protective covers. Short-circuit or electric shock may result. Refer servicing to authorized service personnel only.
- The system contains button battery; unauthorized personnel are **NOT** allowed to repair or replace the battery.
- Before cleaning the system, shut down the system and unplug the power cord. Otherwise, electric shock may result.
- Keep the system dry all the time; avoid fast moving the system from a cold place to a warm place. Otherwise, condensation or water droplets may occur, which may lead to short circuit or shock hazard.
- When the non-medical electrical equipment in the system is powered by a removable, multiperture socket with an isolating transformer, the plug must be full-plugged into a standard socket (hospital grade). Professional installer is responsible to comply with the safety requirements.
- All devices (analog and digital) connected to this system must comply with specified IEC standards (e.g. IEC 60950 information technology equipment safety standard and EN 60601-1 medical equipment standard). All configurations must be in accordance with relevant requirements of IEC standards. When using additional peripheral equipment that is to be interconnected by functional connection, the combination is considered to be a medical electrical system. It is your responsibility to comply with EN 60601-1 and test the system to those requirements. If you have questions, contact your sales representative.
- Always use the rear handle to move the system. When moving the system, make sure the casters are unlocked and all cables are put away from the casters. When moving the system for long distance or on inclines, it shall be moved by two people. Avoid ramps that are steeper than 10 degrees to avoid tipping over the system.
- If you have any doubts of the installation or routing of external protective cables, use the internal power supply of the system.
- Sterilization of the machine and accessories is not recommended unless required in the instructions of the accessories.
- The manufacturer shall be notified when the system is scrapped.

CAUTION

- If any part of the system is known or suspected to be defective or incorrectly adjusted, **DO NOT** use the system until it is repaired.
- Use the system in proper environment. **DO NOT** use the system in the cases of direct sunlight, heat source, high humidity, drastic temperature change, dusty or vibration-easily situation.
- **DO NOT** use the system in the vicinity of strong electric field, magnetic field or mobile radio frequency communication equipment, such as mobile phones, radio transceivers, mobile

radio transmitters, etc. Otherwise, poor performance or even malfunction may result.

- When using movable multiperture socket, qualified, safe products with grounding protection should be selected, and the maximum allowable load should not exceed the maximum power of the system.
- DO NOT connect non-system components of electrical equipment to movable multiperture sockets; otherwise it may cause interference, overload and other risks.
- DO NOT place movable multiperture sockets on the ground.
- When there is a large temperature difference in the operating environment of the system, the system should be vacant for 4 hours before the first power-on to keep the temperature and humidity reach a balance within the system.
- The system must be installed and set up by the manufacturer's authorized or trained personnel. Unauthorized personnel may not disassemble, install or misuse the system.
- Shut down the system and unplug the power cord before moving the system.
- Check the casters for obvious damage or malfunction before moving the system.
- Avoid large vibration during transportation. Mechanical parts damage may result.
- DO NOT lean or sit on the control panel. Function button damage may result.
- DO NOT place any object on the control panel to prevent them from falling and causing damage.
- DO NOT block the air filter or the air outlet. Otherwise, the internal temperature of the system may rise, causing fire, personal injury and other potential hazard.
- If the system triggers the shutoff protection, it indicates the malfunction of the system or peripheral equipment. Contact manufacturer's Customer Service Department or sales representative.
- Maintenance shall be taken regularly to ensure the performance of the system, and ensure that the system is well grounded and meets the safety requirements.
- Changes and additions to the system should be conducted only by personnel authorized by the manufacturer.
- The manufacturer may provide, upon request, block diagrams, lists of spare parts, descriptions, adjustment instructions, or similar information which helps qualified technical personnel in repairing those parts of the system which have been defined as repairable.

1.1.1.2 Accessories Safety



- Use only approved accessories, e.g. probes, peripheral equipment or cables.
- Ultrasound probes are intended for use by qualified specialist staff only. Physicians who use this system for biopsy must undergo

professional ultrasound guidance training and strictly observe the operation requirements of biopsy in order to avoid unnecessary harm to animals.

- DO NOT immerse any probes beyond the specified cleaning or disinfection level showed in “12.1.4 Probe Disinfection”.
- Never make conducting solution contacts with probes.
- Printer can be used in an animal environment.
- For the safe use and maintenance of the printer, please refer to the printer manual.
- Thermal printer shall be only powered by external power source.
- Ensure that the probe and cable are normal before and after performing an ultrasound exam. Use the probe with care. Stop use immediately if the probe appears to be malfunctioning.
- Pay attention to careful use of cable, check the cable before and after use. If there is any damage, stop using the system immediately.
- Never attempt to strike or damage the surface of transducer. Otherwise, electric shock may result when using.
- Components connected to the system shall meet the safety requirements in this manual.

CAUTION

- The system and accessories are not disinfected when delivering. Before using probe and biopsy bracket, disinfect them according to the method provided in their instructions.
- Always inspect whether the edge of the probe is too sharp or the surface is too rough before using the probe. If so, replace the probe to avoid damaging sensitive tissue.
- Use the probe with care, and place the probe properly in the probe holder after use. When out of service for a long time, the probe should be protected by a silicone probe cap.
- DO NOT disconnect probe when scanning. Otherwise, system damage may result.
- Normally, there is no risk of burns when using this system; however, if the probe is placed in the same part of the animal's body for a long time, burns may result. Under the condition of obtaining effective images, shorten the inspection time as possible.
- Shut down the system before plugging or unplugging the system or other peripheral equipment (such as printers). Otherwise system damage may result.
- Always use approved, sterile coupling gel. Read the instructions of the coupling gel carefully before use.
- Remove the coupling gel from the probe thoroughly after each use. Otherwise, moisture in the coupling gel may affect the safety and performance of the probe.
- After cleaning or disinfecting accessories, the chemical reagents or odors must be completely removed.
- Never use foot switch in operating room.

1.1.1.3 Software Safety

- CAUTION**
- To ensure the security of data, users must back up to external storage media when recording important data (such as hospitals, animal data, etc.), for the data stored in the system may be lost due to abnormal operation or failure.
 - DO NOT shut down the system when printing, saving or loading data; otherwise, data will be lost.
 - Improper power failure may result in damage to the drive or system.
 - Attempt to power the system on again at least 5 minute later after each shutting down. Otherwise, system malfunction may result.
 - DO NOT run non-system software on your system computer.
 - Before using the USB flash disk, please format the USB flash disk to prevent computer viruses from intruding the system.

1.1.1.4 Biological Hazard





- To ensure the safety of animals and inspectors, it is forbidden to directly touch samples, mixtures and waste liquids. Please use protective materials (gloves, probe sheath, etc.) during operation, and perform disinfection steps as needed.
- If the sample contacts with skin inadvertently, you must immediately stop operating and notify your physician.
- Some disinfectants have strong acidity or alkalinity. Please use them carefully to prevent direct contact with hands and clothes. If hands or clothes are inadvertently exposed to disinfectants, wash them with soap and flowing water immediately; if disinfectants enter eyes inadvertently, wash them with plenty of clean water immediately and consult an ophthalmologist.
- Disinfectants, intensive cleaning agent and waste liquids must be disposed of as bio-hazardous material in accordance with local standards. Consult the relevant disinfectant manufacturer or distributor for details.
- Probes used on animals with transmissible spongiform encephalopathy (e.g. Mad Cow Disease) must be disposed of. Otherwise, it may infect the animals and operators. There is no method to clean, disinfect the probes used by prion disease patients currently.
- Follow all internal infection control procedures applicable to personnel and systems.
- Disposable biopsy bracket must be disposed of as infectious waste.
- Disinfect the reusable biopsy bracket before storing it.

1.1.2 Labels and Symbols

The following table describes the important information of labels and symbols used on the equipment.

Table 1 Labels and symbols

Labels/symbols	Description
Tag	Tag includes the following information: • The name and address of the manufacturer • Date of manufacture • Model and Serial Number • Electrical rating (voltage, frequency)
	Type BF applied part
	Important information concerning the safe operation
	Dangerous voltages
	Equipotentiality
	Alternating current
	Power on/ off switch
	USB port
	Ethernet connection
	Manufacturer
	Date of manufacture
	Serial number
	Refer to user manual/booklet
	Fragile, handle with care

Labels/symbols	Description
	Keep dry
	Away from sunlight
	Keep facing up
	Temperature range (transport and storage)
	Warning hands pinching
	Medical device
	DO NOT operate the system in the presence of flammable gases or anesthetics or ethyl alcohol. Explosion may result.
	No heavy load on top
	Not to be vertically stacked
	Indoor use only
	Waste electrical and electronic equipment
	Relative humidity range (transport and storage)
	Atmospheric pressure range (transport and storage)
	Nonionizing electromagnetic radiation
	Chinese Environmentally Friendly Use Period symbol

1.2 Application of Acoustic Power

Although it is generally believed that diagnostic ultrasound is safe, there are still studies confirming that there is a risk of damage when high-intensity ultrasound passes through body tissues. Therefore, the operator must follow the ALARA principle when using the ultrasonic diagnostic equipment and use the ultrasound with care.

1.2.1 ALARA

The guiding principle for the use of diagnostic ultrasound is defined by “ALARA principle” (As Low As Reasonably Achievable). That is, by keeping ultrasound intensity as low as possible while obtaining diagnostic images.

The ultrasound intensity depends on the intensity and exposure time of irradiation.

The ultrasound intensity required differs among application modes and animals.

Less ultrasonic power can only obtain low-quality images, which affects the reliability of the diagnosis; while using overdose ultrasonic power increases the risk of bioeffects.

Therefore, it is operator’s responsibility to reconcile ultrasonic power with diagnostic image quality. That is, to obtain qualified images while minimizing the ultrasonic bioeffects.



Warning Special attention should be paid to the ALARA principle in obstetric exam, as any potential bioeffect can have a significant impact on the embryo or fetus.

CAUTION

- Operators should always follow the ALARA principle to ensure the image quality and keep the referencing index and exposure time at lowest level.
- It is important for operators to master the function of the system and observe the acoustic output referencing index reading all the time.

1.2.2 Bioeffect

Ultrasound produces two types of bioeffects, thermal and mechanical.

1.2.2.1 Temperature Index (TI)

The TI informs the operator about the potential for temperature rise in body tissue. It is an estimate of temperature rise in body tissue with specific properties. And temperature rise is influenced by factors such as tissue type, vascularity, operation mode, and others.

There are three types of TI. The system only displays one index at a time. The operator should choose the appropriate index to display according to the actual application location:

- The soft tissue thermal index (TIS) is suitable for abdominal and cardiac application. It indicates the potential for temperature rise in homogeneous tissue.
- The bone thermal index (TIB) is suitable for obstetric (mid-late pregnancy) or pediatric (newborn head) applications. It indicates the potential for temperature rise of bones or at near soft tissue.

- The cranial thermal index (TIC) indicates the potential for temperature rise of bones or at near soft tissue.

1.2.2.2 Mechanical Index (MI)

The MI informs the operator about the possibility for mechanical bioeffect occurrence. It is an estimate of damage in body tissue due to cavitation.

The higher the MI value the greater the possibility of mechanical bioeffect result.

NOTE: When gas and soft tissue exist at the same time, special attention should be paid to setting the MI value to a lower level.

1.2.3 Output Display

The system displays two basic index of Acoustic Output.

TI includes TIS, TIB and TIC. Each probe has a set of appropriate default options.

A TIS, TIB or TIC is displayed by probe and application mode chosen and the increment is 0.1 on the system.

The MI ranged from 0~1.9, the increment is 0.1.

A lower TI/MI index signifies a lower bioeffect. Operators should take TI and MI values as a reference when applying the ALARA principle.

1.2.4 Probe Surface Temperature

The surface temperature of the transducer should not exceed 43°C to ensure the safety of animals.

1.2.5 Acoustic Power Control

The acoustic power can be controlled through three ways:

1.2.5.1 Direct Control

The direct control is to adjust the acoustic power by rotating the knob under **[A.Power]**.

The maximum value of acoustic output in any mode should not exceed the limit value of acoustic output (MI limit value is 1.9, $I_{spta,3}$ limit value is 720 mW/cm²).

1.2.5.2 Indirect Control

Indirect control is mainly performed by adjusting image parameters to control the acoustic power. Parameters that affect acoustic power include: imaging mode, probe and its frequency, position and number of focus, image depth, and PRF.

1.2.5.3 Receiver Control

The receiver control only affects the receiving mode of the ultrasonic wave, and does not

affect the acoustic output while improving the image quality. The operator can optimize the image quality by adjusting the gain, TGC, and dynamic range to obtain effective diagnostic image with the minimum acoustic output.

Receiver control is recommended before direct control and indirect control.

Chapter 2 System Overview

2.1 Application Range

The device is suitable for clinical ultrasound examination for dogs, cats, equine, bovine and ovine.

2.2 Contraindications

None.

2.3 System Configuration

2.3.1 Standard Configuration

- Console
- CD/DVD drive
- Accessories
 - User manual*1
 - Warranty card*1 (with certificate of conformity)
 - Power cord*1

2.3.2 Optional Probes

Imaging probes used for exam may affect the RF emissions of the system.

The following probes have been tested in accordance with the requirements of the CISPR 11 and confirmed to meet the radiation standards of Group 1 Class A products.

Table 2 Optional Probes

No.	Probe Model	Nominal/ Testing Frequency (MHz)	Frequency Range (MHz)	Probe Type	Intended Use	Region Applied
1	3C5PD	3.5	1.0-7.5	Convex Array	Cardiology, abdomen, reproduction, vascular, and small parts	Surface
2	3C5PDS	3.5	1.0-7.5			

No.	Probe Model	Nominal/ Testing Frequency (MHz)	Frequency Range (MHz)	Probe Type	Intended Use	Region Applied
5	7L4PD	7.5	4.2-15.0	Linear Array	Abdomen, vascular, small parts, nerve, and musculoskeletal	Surface
6	10L2PD	10.0	4.2-16.0			

10	3P2PA	3.0	1.0-6.5	Phased Array	Cardiology and abdomen	Surface
11	5P1PA	5.0	2.5-13.0			

2.3.3 Optional Accessories

Table 3 Optional Accessories

Item	Service Life
Battery	About 500 times
Printer	About 5 years
Foot switch	About 2.5 years
Gel warmer	About 10 years
ECG lead	About 5 years
Probe	About 3 years

2.4 System Components

2.4.1 Console

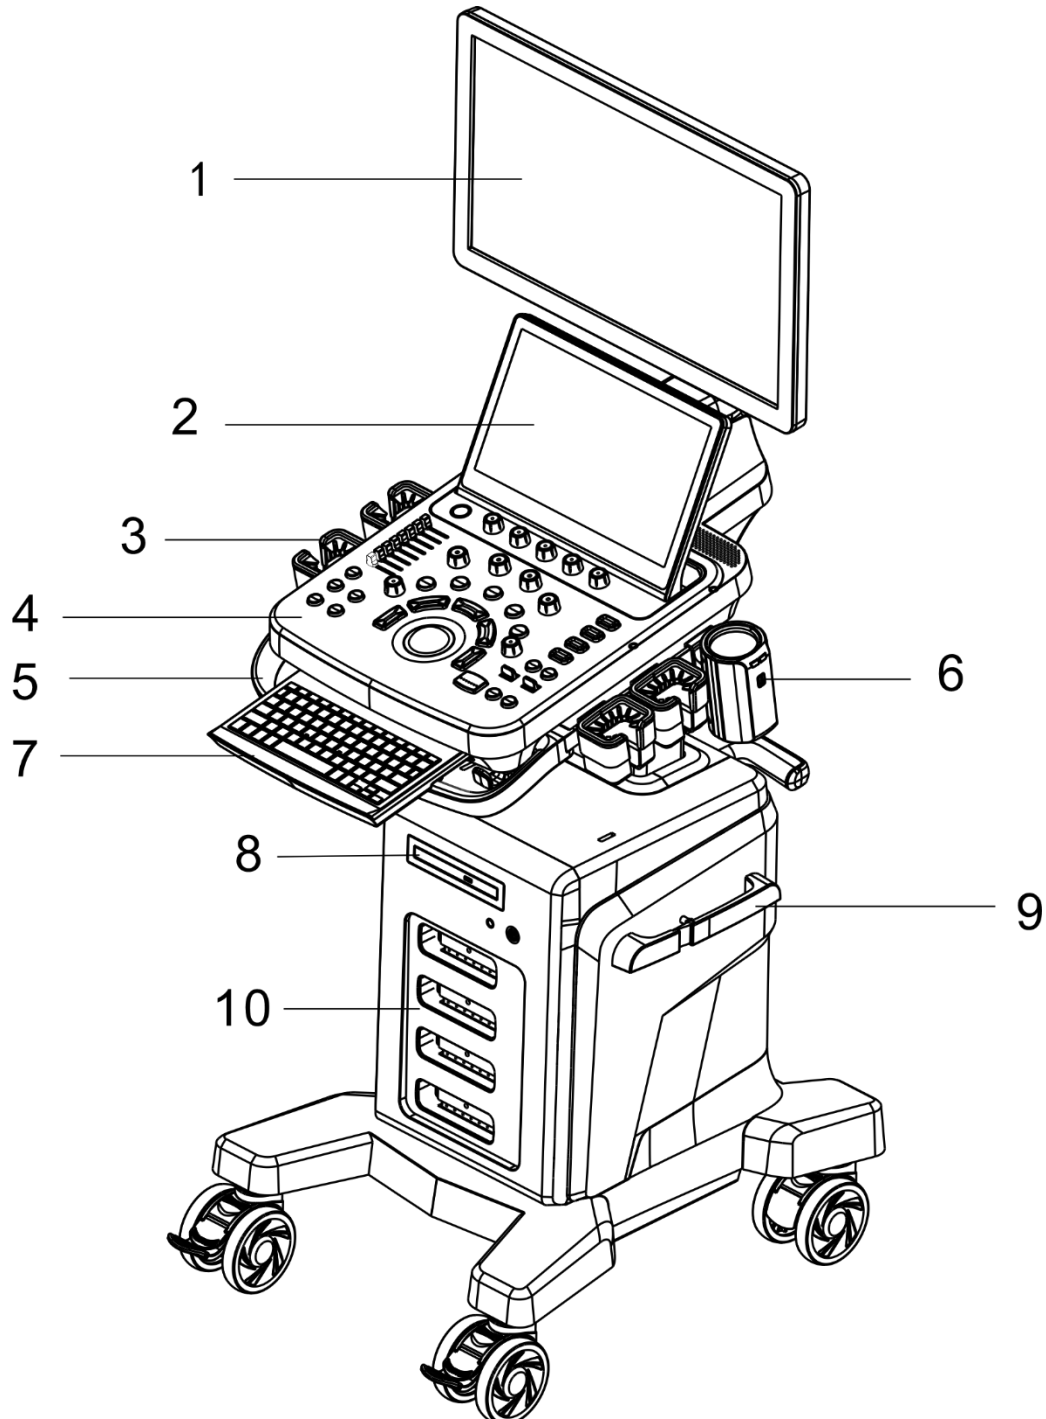


Figure 1 Front View

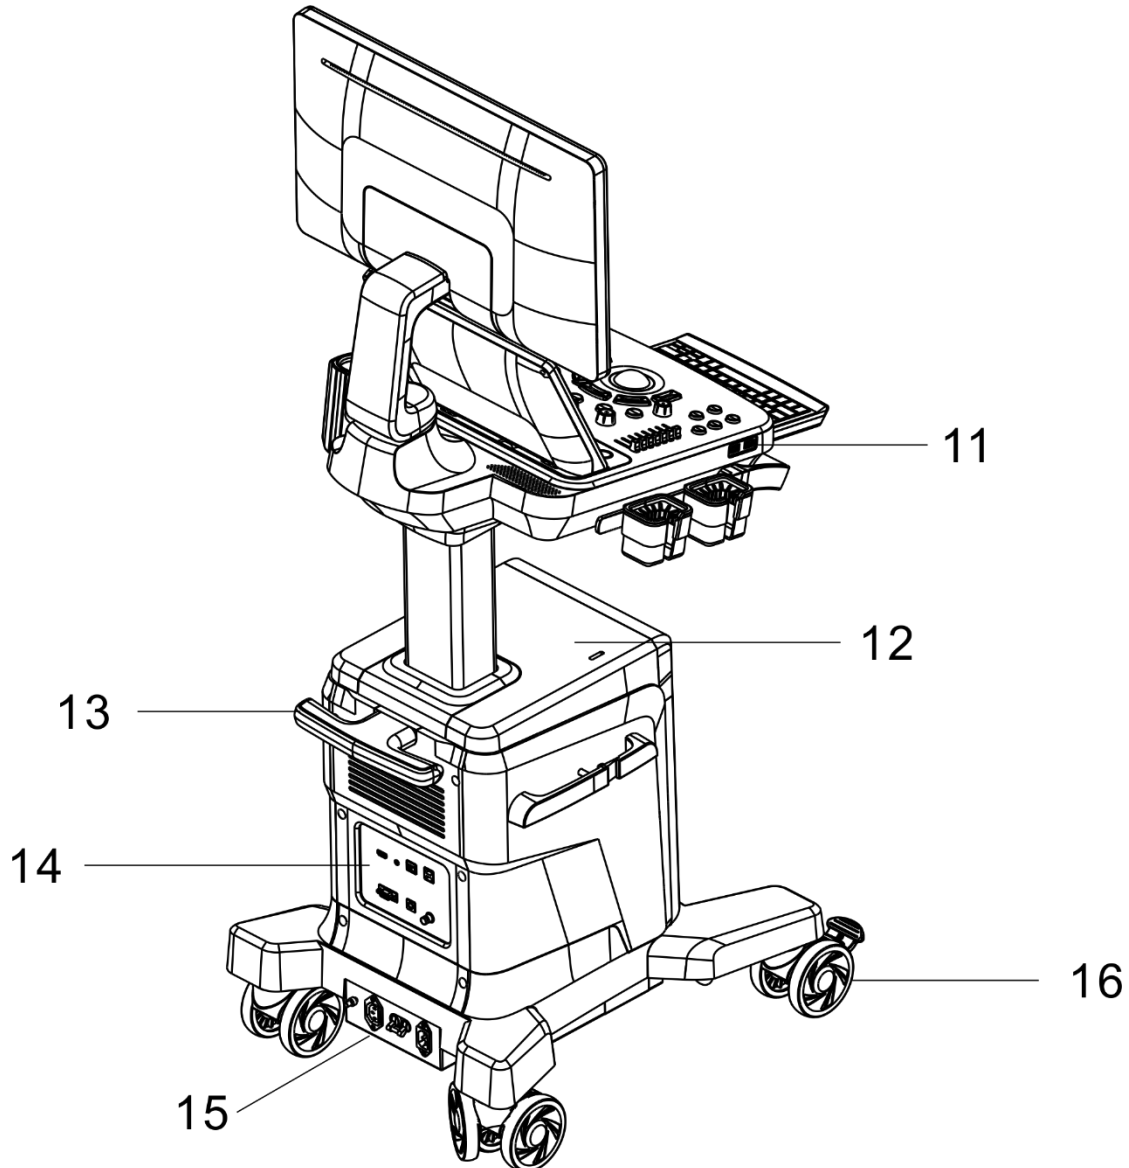


Figure 2 Back View

Table 4 Console

No.	Item	Function
1	Monitor	Display all user interfaces.
2	Touch Screen	Provide system human-machine interface to facilitate the operation and control.
3	Probe Holder	Used for fixing a probe.
4	Control Panel	Provide system human-machine interface to facilitate the operation and control.
5	Front Handle	Used for moving the system and adjusting the rotation angle of control panel.
6	Gel warmer (optional)	Used for warming the coupling gel.

No.	Item	Function
7	Keyboard	Used for text entering.
8	CD/DVD drive	Used for ultrasonic image burning. (Optional)
9	Hanger	Used for fixing cables.
10	Front Panel	Probe receptacles. Refer to “2.4.5 Front Panel” for details.
11	USB Port	Connects an USB device.
12	Printer Storage	Used for printer storage.
13	Rear Handle	Used for hanging the cable and lifting the system.
14	I/O board	Used for connecting peripherals and accessories. Refer to “2.4.6 I/O Board” for details.
15	Power Supply Panel	Electrical port panel. Refer to “2.4.7 Power Supply Panel” for details.
16	Caster	Used for moving or fixing the system.

2.4.2 Control Panel

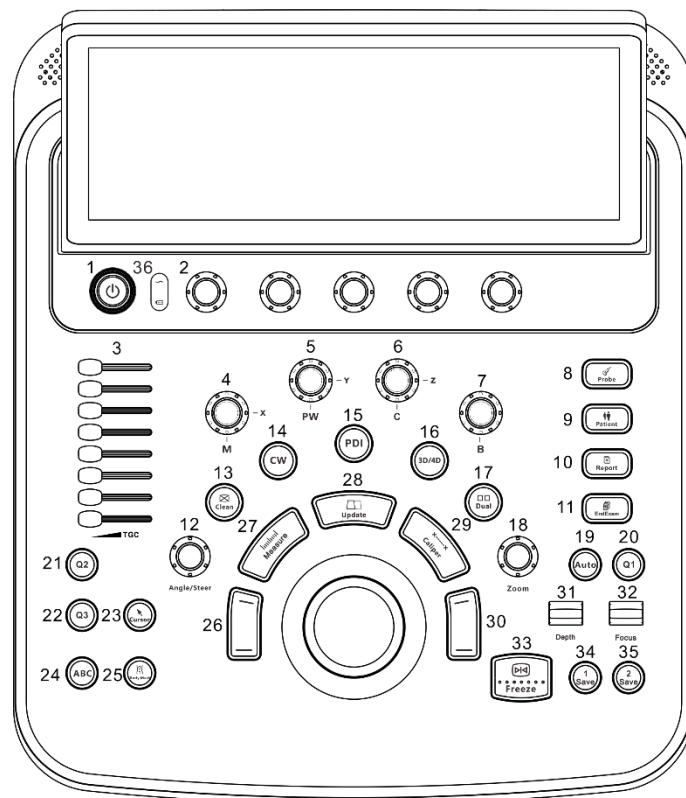


Figure 3 Control Panel

Table 5 Control Panel

No.	Icon	Description	Function
1		Power switch	Power on/ off the system.
2	/	Touch screen knob	Adjust the parameters corresponding to the touch screen.
3	TGC	TGC sliders	Move left and right to adjust depth gain.
4	M	M mode knob	Press to pre-activate M mode; double-press to enter M mode. Rotate to adjust gain in M mode.
5	PW	PW mode knob	Press to pre-activate PW mode; double-press to enter PW mode. Rotate to adjust gain in PW/CW mode.
6	C	Color mode knob	Press to enter Color mode. Rotate to adjust gain in Color/PDI mode.
7	B	B mode knob	Press to enter B mode. Rotate to adjust gain in B mode.
8	Probe	Probe/Exam switch button	Toggle probe and exam mode.
9	Patient	Animal information button	Enter / exit the Animal Information screen.
10	Report	Report button	Enter / exit the Report screen.
11	EndExam	EndExam button	End the current exam.
12	Angle/Steer	Angle/Steer knob	Adjust the angle / steer angle.
13	Clear	Clear button	Clear the measurement, comments and body mark.
14	CW	CW mode button	Press to pre-activate CW mode; double-press to enter CW mode.
15	PDI	PDI mode button	Press to enter PDI mode.
16	3D/4D	3D/4D button	Press to enter the 3D standby mode; press again to enter the 4D standby mode. Toggle between 3D and 4D modes. (Reserved

No.	Icon	Description	Function
			function)
17	Dual	Dual display	Activate the dual display function. Or toggle between the two image states.
18	Zoom	Zoom knob	Rotate the knob to zoom in/out the full-ultrasound image. Press the knob and then rotate to zoom in/out local ROI box.
19	Auto	Auto button	Press to activate the Auto Optimization function.
20	Q1	Customize Shortcut Button	User-defined button. You can customize its function depending on your needs.
21	Q2	Customize Shortcut Button	Enter TDI mode by default. You can customize its function depending on your needs.
22	Q3	Customize Shortcut Button	User-defined button. You can customize its function depending on your needs.
23	Cursor	Cursor button	Display or hide a cursor.
24	ABC	Text button	Activate / exit text function.
25	Body Mark	Body Mark button	Activate / exit body mark function.
26		Left set button	Press to confirm the operation.
27	Measure	Measure button	Activate / exit application measurement and calculation functions.
28	Update	Update button	In M pre-activation mode, press this button to switch to B+M mode. In the B+PW/B+CW mode, press this button to switch between the PW/CW image and the B mode image.
29	Caliper	Caliper button	Activate / exit general measurement function.
30		Right set button	Press to confirm the operation.
31	Depth	Depth slider	Move up and down to adjust the imaging depth.

No.	Icon	Description	Function
32	Focus	Focus slider	Move up and down to adjust the focus position.
33	Freeze	Freeze button	Press this button to freeze the current image and press again to resume real-time status.
34	Save 1	Image save button	Press this button to save the current frame image by default. You can customize its function depending on your needs. Refer to “4.2.5 Customize” for details.
35	Save 2	Cine save button	Press this button to save the set cine by default. You can customize its function depending on your needs. Refer to “4.2.5 Customize” for details.
36		Power indicator	Indicates the power status. When AC power supply connected, the AC indicator lights up; when AC power disconnected, the AC indicator light turns off. When using battery power, the battery indicator light lights up (green indicates full charge; orange indicates charging); When there is no battery or no AC power, the battery indicator light turns off.

2.4.3 Trackball

Use the trackball and **[Set]** button to control the screen directly and easily.

Function	Description
Move	Roll the trackball to move the cursor.
Click / Select	Use the trackball to move the cursor over the item, image, or annotation you want to select and press the [Set] button.
Drag	1) Click the image, or annotation you want to move and press the [Set] button. 2) Roll the trackball to move the image or annotation to the desired location. 3) Press the [Set] button again.
Adjust ROI	1) Roll the trackball to adjust the size of ROI frame. 2) Press the [Set] button.

2.4.4 Keyboard

The keyboard is located under the control panel.

Eject the keyboard: Press the keyboard edge in and let go, the keyboard will pop up

automatically, pull the keyboard out until it clicks to fix the keyboard.

Close the keyboard: push the keyboard in until it clicks to secure the keyboard.

The keypad consists of numbers, letters and function keys for text entering, which is the same as the computer keyboard.



Figure 4 Keyboard

Table 6 Keyboard Description

No.	Key	Function
1	Esc	Back to Home screen.
2	Help	Open / close accompanying help documents.(Reserved function)
3	Station	Enter / exit Work Station screen.
4	Setup	Enter / exit System Setup screen.
5	Q4~Q8	User-defined keys.
6	FZoom	Activate / toggle / exit full-screen zoom function.
7	ECG	Activate / exit ECG function.
8	Biopsy	Activate / exit biopsy function.
9	QSave	Save the current image parameters as a preset for the next exam.
10	1~9	Number key.
11	Tab	Jumps to next menu item.
12	Caps Lock	Toggle between uppercase and lowercase.
13	Shift	Key combination. Used together with other keys.
14	Ctrl	Key combination. Used together with other keys.
15	Fn	Key combination. Used together with other keys.
16	Alt Gr	Key combination. Used together with other keys.
17	Del	Delete the character after the cursor.

No.	Key	Function
18	A~Z	Character key.
19	Space / Text	Insert a space / activate comments.
20	Body Mark	Activate / exit body mark function.
21	Arrow	Activate / exit arrow annotation function.
22	↑←↓→	Move the cursor position by character.
23	Enter	Move the cursor to the next line of text or the input box.
24	Special character	Special character key.
25	Back	Delete the character before the cursor.
26	Delete Text	Delete all text annotation on the screen.

2.4.5 Front Panel

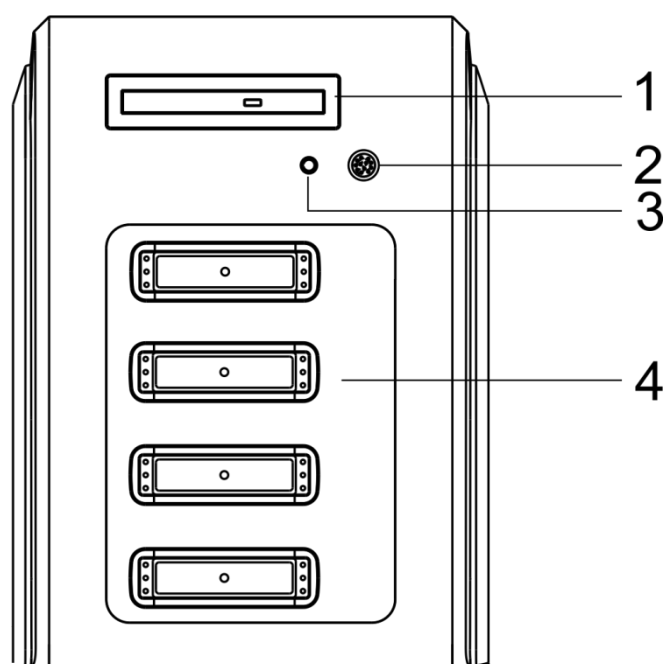


Figure 5 Front Panel

Table 7 Front Panel Description

No.	Name	Function
1	CD/DVD-RW	Used to back up animal data and images.
2	ECG lead port	Used to connect the ECG cable.
3	Pencil probe port (Reserved)	Used to connect pencil probe.
4	Probe receptacles	Used to connect ultrasonic probes.

2.4.6 I/O Board

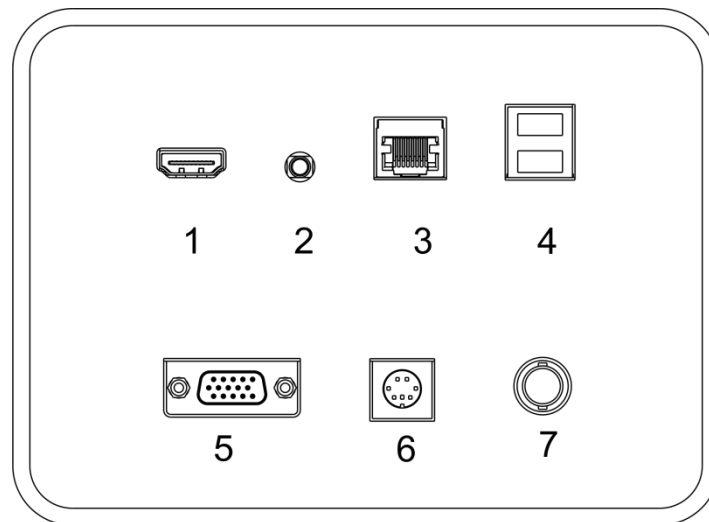


Figure 6 I/O Board

Table 8 I/O Board Description

No.	Item	
1	HDMI	Compatible equipment must comply with EN 60601-1
2	Printer remote control	Sony UP-25MD, Sony UP-X898MD or other printers that comply with EN 60601-1 standards
3	Network port	/
4	USB port	USB flash drive: Sandisk GZ600 or other products that comply with CE standards Foot switch: KACON/HRF-M2Y-U
5	VGA port	Compatible equipment must comply with EN 60601-1
6	S-VIDEO output	Compatible equipment must comply with EN 60601-1
7	VIDEO output	Compatible equipment must comply with EN 60601-1

- NOTE:**
- S-VIDEO port is recommended.
 - To ensure image quality, make sure that the resolution of the external video output device (HDMI/VGA) is 1920*1080.

2.4.7 Power Supply Panel

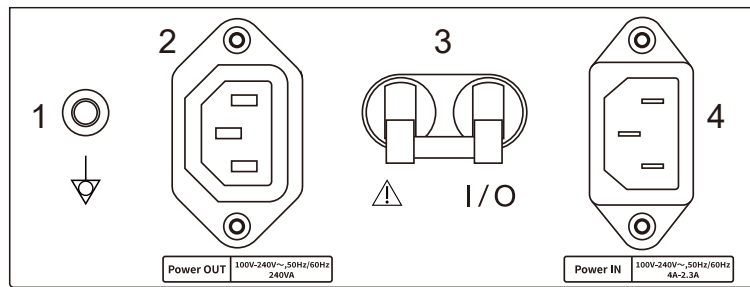


Figure 7 Power Supply Panel

Table 9 Power Supply Panel

No.	Item	Description
1	Equipotentiality	Equipotential terminal.
2	Power outlet	AC power output port.
3	Circuit breaker	Turn on/off the power supply.
4	Power inlet	AC power input port.

Chapter 3 Preparing the System

3.1 Moving the system

Care must be taken when moving the system and the specifications of this section must be strictly followed.

3.1.1 Transporting

When transporting the system, make sure the packaging is in good conditions and follow the precautions below:

- NOTE:**
- Strictly comply with the graphic symbols on the packaging when transporting the system by vehicle.
 - The delivery vehicle must be a van.
 - Do not stay in the sun, rain or snow without any covering when loading or unloading the system.
 - DO NOT transport the items which may damage the system together. DO NOT put any heavy items on the packaging.
 - When using a vehicle for transportation, make sure that the vehicle can bear the system as well as the passenger's weight.
 - If lifting equipment is used, make sure that the load capacity of the lifting equipment can bear the weight of the system. (With all components, the weight of the system is about 65kg)

3.1.2 Moving

To move the system, perform the following steps:

1. Before moving the system, make sure that the system is powered off and the power cord is unplugged.
2. Properly fix all cables, probes and accessories to prevent tripping hazard when moving the system.
3. Unlock the casters.
 - Step on the **[ON]** pedal to lock the casters. The system cannot be moved.
 - Step on the **[OFF]** pedal to unlock the caster. The system can be moved flexibly.
4. Firmly hold the rear handle of the system with two hands when moving the system.

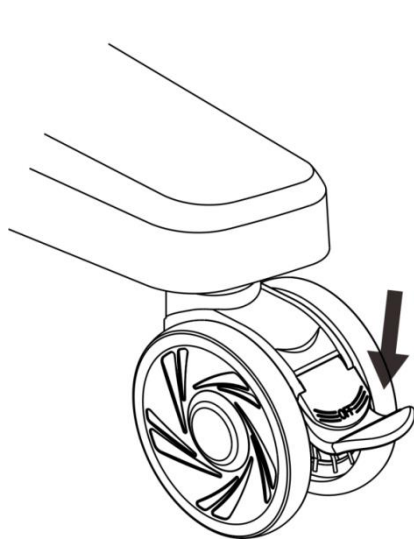


Figure 8 Lock the casters

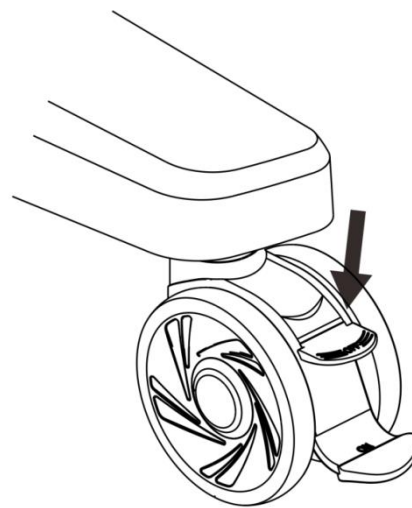


Figure 9 Unlock the casters



Warning

Fail to move the system as described above may led to a tipping hazard, causing possible animal or operator injury and damage to the system.

NOTE:

- **Avoid to passing slopes over 10°. If have to, need to be moved by two people. Always moving the system with the rear handle.**
- **If necessary, use the rear handle of the console to lift the system gently instead of lifting the system directly.**
- **Before moving the system, please check the casters for obvious damage or poor rotation.**

3.2 Positioning

To position the system, perform the following steps:

1. Position the system on a level, anti-slip surface. Leave at least 20 cm of space on the back and left and right sides of the system.
2. Properly place all power cords and cables to prevent tripping hazard.
3. After positioning the system at a properly place, lock the casters to prevent a slip hazard.



Warning

DO NOT place the system on a slope or a slippery surface to prevent a tipping hazard which causes possible animal or operator injury and damage to the system.

3.3 Connecting the System

The system supports external power supply and battery power supply. Normally, it is recommended to work with an external power supply. In special cases, such as sudden power failure or easy system movement, battery power supply is preferred.

3.3.1 External Power Supply

The system power must be supplied from a properly rated outlet as described on the Power Supply Panel.

To connect external power supply, perform the following steps:

connect the power inlet of the power Supply Panel and a hospital grade grounded power outlet with the power cord.

3.3.2 Battery Power Supply



Warning

- **Battery can only be disassembled or installed by professionals. Battery replacement by personnel without adequate training can result in fire or explosion hazards caused by over-temperature. Disassembly and assembly by user will void the warranty. If the battery fails or needs to be replaced, please contact the manufacturer or your sale-representative.**
- **If you do not use the system for a long time in battery mode, please shut down the system. Frequent charging and discharging will impact the service life of batteries.**

3.3.2.1 Battery Charging and Use

The battery is a rechargeable lithium-ion battery.

When an external power source is connected, the battery will be charged automatically when the battery power is not full.

The system switches to battery power supply automatically when external power source is removed. Fully charged battery will give about 1 hour of use.

3.3.2.2 Battery Status

Battery status is indicated by icons on the status bar.

Table 10 Battery Status Icons

Icon	Description
	Battery level 80%~100%
	Battery level 60%~80%
	Battery level 40%~60%
	Battery level 20%~40%
	Battery level 10%~20%
	Battery level below 10%
	Charging

When the battery power is 10%, a system prompt will be displayed, which disappears after

5 seconds.

When the battery power is 5%, a system prompt will be displayed. Click **[OK]** or **[Cancel]** to hide the prompt.

3.3.2.3 Battery Maintenance

It is recommended to perform a complete discharge/charge cycle when the battery is used for the first time or not used for more than 3 months.

To perform a complete discharge/charge cycle:

1. Allow the battery to discharge completely until the system turns off.
2. Full charges the battery.
3. Repeat step 1~2 if necessary.

3.3.2.4 Battery Recycling

Replace and properly recycle the battery when it is obviously damaged or exhausted. Follow the corresponding regulations when disposing the used batteries.

3.4 Power On/ Off the System

3.4.1 Power on

- CAUTION:**
- Do not power on the system without probe connected.
 - If an abnormal power interruption occurs during the last system operation (such as a sudden interruption of AC power), you may have to wait longer 30~60s than usual to reboot the system.
 - System can be rebooted 5 minute later of power off. Otherwise system failure may result.
- NOTE:**
- First power-on is recommended to be done by the authorized personnel.
 - Make sure that the power cord is connected to the system and fully plugged into an appropriate grounded power rating outlet.
 - Do not place the system in a location where it is difficult to disconnect the power supply plug.

To power on the system, perform the following steps:

1. Push up the circuit breaker located on the Power Supply Panel to connect power supply.
2. Press the power switch “” located on the upper right section of the control panel to startup the system and the power indicator lights up.
3. A boot screen appears, and the Home screen displays after startup.
4. After initialization has been completed, refer to the following items for startup check. If there is any abnormality, please contact your sales representative or

the customer service department of the manufacturer.

Table 11 Checking List

No.	Item
1	Abnormal sound, smell, or overheating.
2	Error message.
3	Discontinuous display or abnormal dark area on the 2D image.
4	When the probe is connected to the system, monitor that the surface temperature of the probe all the time to avoid abnormal heat that may burn the animal.
5	The buttons and knobs of the control panel are fully functional.
6	The system time displays correctly.

3.4.2 Power off

To shut down the system, perform the following steps:

1. Press the power switch “” located on the upper right section of the control panel.
2. A confirmation prompt pops up, select **[Shutdown]** to power off the system.
3. When the power indicator lights out, the shutdown is completed.
4. Remove the plug from the wall outlet as needed.

CAUTION:

- Never attempt to shut down the system while the system is in an upgrade or data transfer process.
- DO NOT remove U disk or cut down the power during upgrading.
- End the current exam before shutting down the system.
- DO NOT cut down the power before the shutdown procedure is completed. Files damaged and animal data loss may result.

NOTE:

- If the system fails to shut down normally, unplug the power cord to force the system to shut down.
- It is not recommended to power off the circuit breaker or to remove the power plug directly for doing this may cause damage or loss of animal data.
- If the system is not used for a long time, disconnect the external power supply and turn off the circuit breaker, disconnect all peripheral equipment after shutting down the system.

3.4.3 Standby

Without any operation for a period of time, the system will enter standby mode. You can set the waiting time to enter the standby mode.

Setting path: **[Preset]** (press <Setup>) → **[System Preset]** → **[General]** → **[Standby]**, refer to “4.2.2 General” for details.

3.5 Mechanical Adjustment

Before starting the exam, you can adjust the monitor, control panel, and touch screen for easy viewing.

- NOTE:**
- Lock the caster before mechanical adjustment.
 - Be careful to prevent crushing your hands when making the mechanical adjustment.

3.5.1 Adjust the Monitor

The horizontal angle and vertical angle of the monitor can be adjusted. The display parameters of the monitor can also be adjusted for optimal display performance.

3.5.1.1 Adjust the Horizontal Angle

Grab the edge of the monitor with two hands and rotate the monitor horizontally.

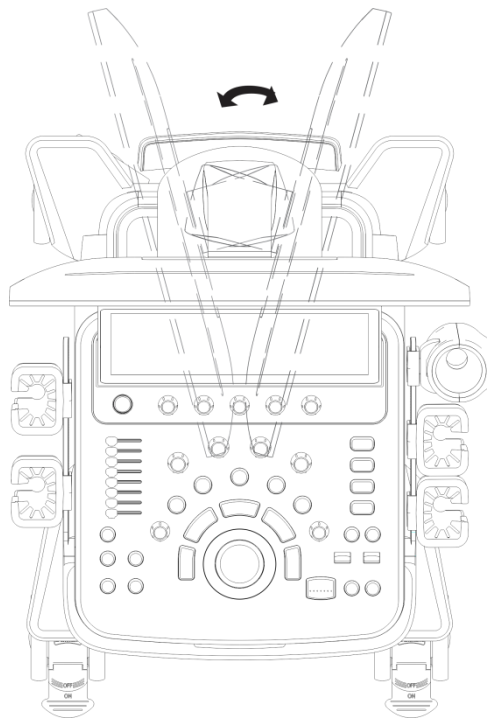


Figure 10 Adjust the Horizontal Angle

3.5.1.2 Adjust the Vertical Angle

Grab the top and bottom of the monitor with two hands and tilt the monitor up and down.

- NOTE:**
- Be careful to prevent crushing your hands when adjusting the monitor.
 - When transporting or moving the system, tilt the monitor to the

horizontal position to avoid damage to the screen.

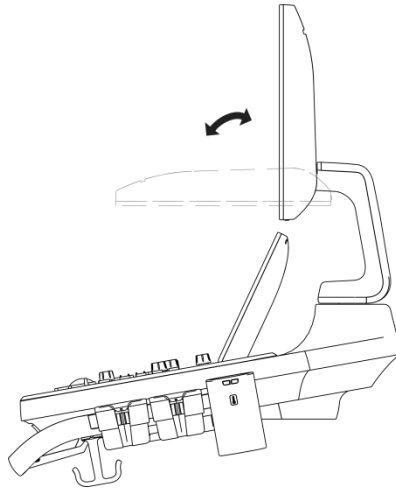


Figure 11 Adjust the Vertical Angle

3.5.1.3 Adjust Brightness and Contrast

Monitor's brightness and contrast are two of the most important factors for proper image quality.

NOTE: Do not turn off the monitor during use, as this may result in loss of animal data and need to reboot.

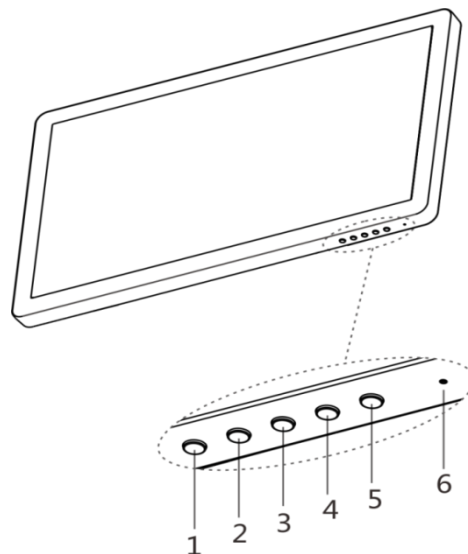


Figure 12 Monitor Control Button

Table 12 Monitor Control Button

No.	Description	No.	Description
1	Menu	2	Enter /Exit
3	Contrast /Decrease	4	Brightness/ Increase
5	Power On/ Off	6	Status Indicator

➤ **Contrast Control**

1. Press **[3]** to activate the contrast control and the contrast bar is displayed in the lower right corner of the screen.
2. Press **[3]** to decrease the contrast or **[4]** to increase the contrast.
3. Press **[2]** to exit the contrast control.

➤ **Brightness Control**

1. Press **[4]** to activate the brightness control and the brightness bar is displayed in the lower right corner of the screen.
2. Press **[3]** to decrease the brightness or **[4]** to increase the brightness.
3. Press **[2]** to exit the brightness control.

➤ **Other Parameters**

Press **[1]** to open the parameter menu.

- NOTE:**
- **Adjust the brightness prior to the contrast.**
 - **After readjust the monitor's brightness and contrast, readjust all preset and peripheral settings.**

3.5.2 Adjust the Control Panel

Grab the rear handle with two hands and rotate the control panel horizontally.

3.5.3 Adjust the Touch Screen

Hold the top and bottom of the monitor with two hands and tilt the touch screen.

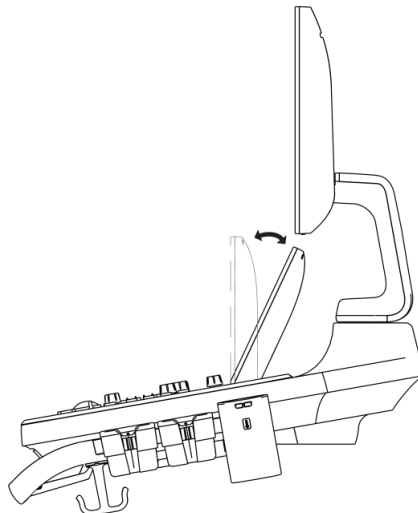


Figure 13 Adjust the Touch Screen

3.6 Connect / Remove the Probe



Warning

- Before connecting or removing the probe, freeze the image or shut down the system power, otherwise the system and probe damage may result.
- Use only probes provided by manufacturer. Using other probes may damage the system and probes and cause unpredictable accidents or malfunctions.
- Before connecting the probe, make sure that the surface, cable and socket of the probe are without cracks or any failure. Electrical shock may result if a defective probe has been used.
- Before connecting or removing the probe, place the probe in the probe holder and fix the probe cable to prevent the probe from accidentally falling.

3.6.1 Connect the Probe

To connect a probe, perform the following steps:

1. Turn the locking handle on the probe connector counterclockwise.
2. Keep the probe cable to the right and carefully insert the probe connector into the probe receptacle completely.
3. Turn the locking handle clockwise to lock in place.

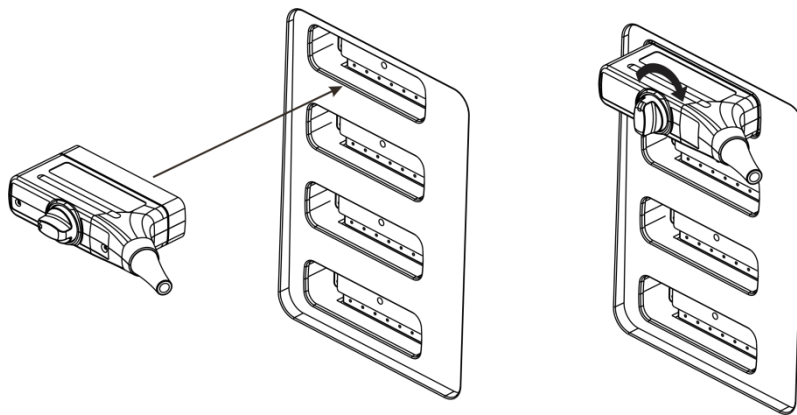


Figure 14 Connect the Probe

3.6.2 Remove the Probe

To remove the probe, perform the following steps:

1. Turn the locking handle counterclockwise to unlock the probe connector.
2. Pull the probe connector straight out of the probe receptacle.

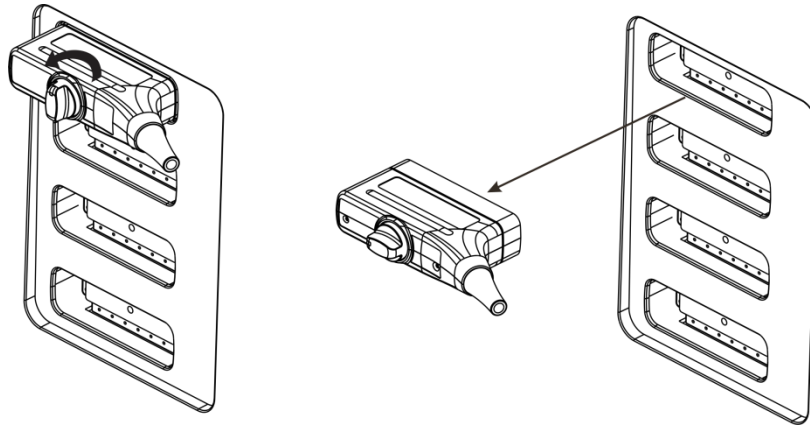


Figure 15 Remove the Probe

3.7 Install the Gel Warmer

Gel warmer is an optional accessory for heating 250 ml of ultrasonic coupling gel to 37°C or 40°C.

Perform the following steps:

1. The warmer's power ports are located at the bottom of both sides of the control panel. Pull out the plug, and connect the power cord of the warmer to the power port of the bottom.
2. Push and fix the warmer into the probe bracket nearby.

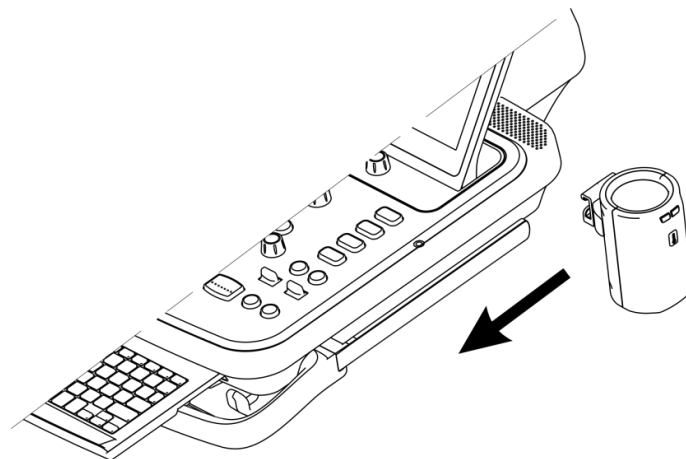


Figure 16 Install the Gel Warmer

3. Press and hold the warmer's power button for more than 1 second to turn on the gel warmer, and the corresponding temperature indicator lights up in green. The coupling gel is heated to 37°C by default.
4. Short press the warmer's power switch to toggle the heating temperature between 37°C and 40°C.

5. Place the 250ml ultrasonic coupling gel into the warmer for heating.
6. Press and hold the warmer's power button for more than 1 second to turn off the gel warmer after use.

3.8 Foot Switch

Foot switch is an optional accessory. Preset its function before use.

Setting path: **[Preset]** (press **<Setup>**) → **[System Preset]** → **[Customize]**, refer to “4.2.5 Customize” for details.

Operation: Connect the foot switch to the system via USB port, and step on the foot switch to perform the corresponding operation.

3.9 Connect the Network

NOTE: To ensure the network security of the system, **DO NOT** connect any external network when using the system normally.

To connect the network, perform the following steps:

1. Connect the network port  of the peripheral connector board and the local LAN port with network cable.
2. Setup the local network.
 - Setting path: **[Preset]** (press **<Setup>**) → **[Network Preset]** → **[Local TCP/IP]**, refer to “4.6 Network Preset” for details.
3. Check the network connection status by the screen status bar.
 -  means successful network connection.
 -  means failed network connection, try to connect again.
 - Place the cursor on the network icon to automatically display the network information.

3.10 Connect Peripheral Device

3.10.1 Connect USB Device

➤ **To connect a USB device:**

1. Insert the USB device into the USB port.
2. After initialization, “” displays on the status bar.

➤ **To remove a USB device:**

1. Move the cursor over the “”, press the **[Set]** button.
2. Select the USB storage device to be removed in the pop-up dialog box and click

[OK] to remove the USB device safely.



Warning

- Do not use USB storage device with unsafe data, otherwise system damage may result.
- Remove the USB device safely. Direct removal may damage the USB device and the system.

3.10.2 Connect Printer

3.10.2.1 Connect Digital Printer

This section takes the HP OfficeJet Pro 8210 as an example. For the connection details for other models of printers, please refer to the printer manual.

To connect a digital printer, perform the following steps:

1. Connect the medical power supply and the printer with the power cable of the printer.
2. Connect the system and the printer with an USB cable.
3. Add print service to the printer.
 - 1) Press <Setup> key to enter the Preset screen. Click [Print Preset] to enter print setting screen.
 - 2) Click [Add Service] to add print service to the printer.
 - 3) Enter the printer service name, select the printer service type, and click [OK].
4. Install the printer driver.
 - 1) The set print service is displayed in the print service list; select the service by pressing [Set] button.
 - 2) Click [Add Printer] and a dialog box pops up.
 - 3) The printer driver path for the connected device will be displayed by URL. Select the desire printer driver and then enter the printer name.
 - 4) Click [OK] to install the driver.



Warning

When using multiple peripherals that are not powered by the auxiliary output of the system, it must be ensured that the total leakage current of the peripherals and the system meets the medical equipment electrical safety standards in relevant areas.

3.10.2.2 Connect Thermal Printer

Please refer to the printer manual for installation details.

Once the printer is connected successful, you can use it after relevant settings.

NOTE: For ease of use, it is recommended that the thermal printer be placed in the printer storage box that comes standard with the system.

3.10.2.3 Connect DICOM Printer

Once the system is connected to the DICOM server and the DICOM print server has been

set up, animal images can be printed remotely. Refer to “11.2.2 DICOM Print” for details.

3.10.2.4 Precautions for Printer

- If any liquid or solid fall into the printer, please stop the operation immediately. Unplug the printer and refer to professional personnel.
- If you do not use the printer for a long time, please unplug the plug from the socket.
- Do not disassemble the printer housing. Only professional personnel can carry out maintenance.
- When the printer is loaded with printing paper, do not move or handle the printer, otherwise it may cause printer failure.
- To prevent internal overheating, leave enough space (at least 10 cm) around the printer.

3.11 ECG

This system supports the ECG function, which is used to collect ECG signals synchronized with ultrasound images during ultrasound exams (mainly cardiac exams). ECG cannot be used for diagnosis or monitoring.




- **ECG cannot be used for cardiac surgery.**
- **Motivated device may affect ECG signals.**
- **Check the ECG leads before operation to ensure that the ECG leads is in conditions. Otherwise, electric shock may result.**
- **Be sure to connect the ECG electrode correctly. Do NOT use ECG leads that are not provided by the manufacturer. Otherwise, electric shock may result.**
- **When connecting the ECG electrode, connect the ECG cable and the ECG lead before placing the ECG electrode on the animal. Otherwise, the animal may get an electric shock.**
- **Do not directly touch the animal's heart with the ECG electrode; otherwise the animal's heartbeat may stop.**
- **If a defibrillator must be used, there must be no ECG adhesive electrode and conductive adhesive before removing the defibrillator electrode.**

3.11.1 ECG Operation

Perform the following steps:

1. Connect the device.
 - 1) Shut down the system and connect the ECG cable to the ECG lead port.
 - 2) Power on the system.
 - 3) Place the ECG electrodes on the animal's body as shown in the following figure.

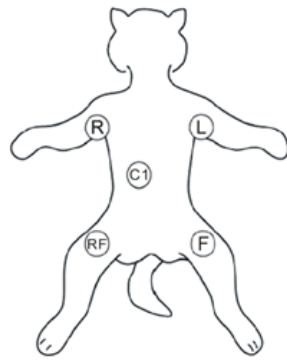

R -- Right foreleg
L -- Left foreleg
RF-- Right hind leg
F -- Left hind leg
C1-- Chest

2. Press the **<ECG>** key on the keyboard to enter the ECG operation screen.
3. Tap **[Start]** on the touch screen to display the ECG signal synchronously, and adjust the corresponding parameters to obtain the best image scanning effect.
4. Freeze the image and observe the replay image and waveform.
5. Tab **[Exit]** on the touch screen to exit ECG screen.

3.11.2 ECG Maintenance

- ECG cables do not require special maintenance, but should be used with care.
- Damaged cables should be replaced promptly.
- Use the electrodes and cables as described.
- Necessary repairs or replacements can only be performed by authorized personnel.

3.12 Screen

3.12.1 Home Screen

The system enters the Home screen by default after power on.

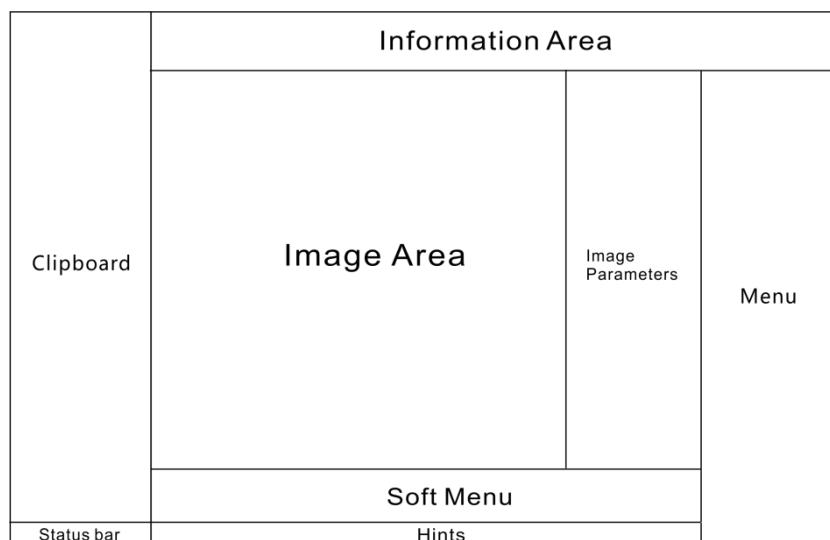


Figure 17 Home Screen

Table 13 Home Screen

Functional Area	Description
Information Area	The information area is located at the top of the Home screen. This area displays information such as LOGO, hospital name, physician, animal information, exam date, current probe model and current exam mode, etc.
Image Area	The ultrasound image area is located in the center of the Home screen. This area displays real-time ultrasound images, probe marks, coordinate axes, focus positions, gray scale bars, and color bars of each exam mode. The parameters such as acoustic power, mechanical index and thermal index are displayed on the upper left of the image area. The cine replay progress bar is displayed under freeze state. The corresponding annotation information is displayed when the text/body mark/arrow annotation functions are activated. The measuring scale is displayed when the measure function is activated.
Image Parameter	The image parameter area is located on the right side of the image area. This area displays the real-time parameters of current mode.
Menu	The menu is located on the right side of the Home screen. This area displays different menus for different screens, including but not limited to image menu, measurement menu, annotation menu and body mark menu.
Soft Menu	The soft menu is located at the bottom of the Home screen. This area displays the options of the current mode and synchronizes the options to the touch screen.
Hints	Display prompt information, help information, or progress status of the current screen.
Status bar	Display icons for current system status, including battery level, power status, network connection status, input method, recycle bin, USB devices, and storage status, etc.
Clipboard	Display a thumbnail of the stored picture under the current exam.

3.12.2 Touch Screen

The touch screen is mainly used to adjust image parameters, switch probes or exam modes, or used as a control interface to facilitate some basic functions.

- CAUTION:**
- Always operate the system in a stable environment. A sharp temperature or humidity change may cause malfunction of the touch screen.
 - DO NOT touch the touch screen with sharp or hard objects.
 - DO NOT expose the touch screen to high voltage or static electricity.

- **DO NOT** expose the touch screen directly to the sun.
- Use your fingers to operate the touch screen and avoid putting too much pressure on the touch screen.
- Keep the screen clean and **DO NOT** stick tape on the touch screen.

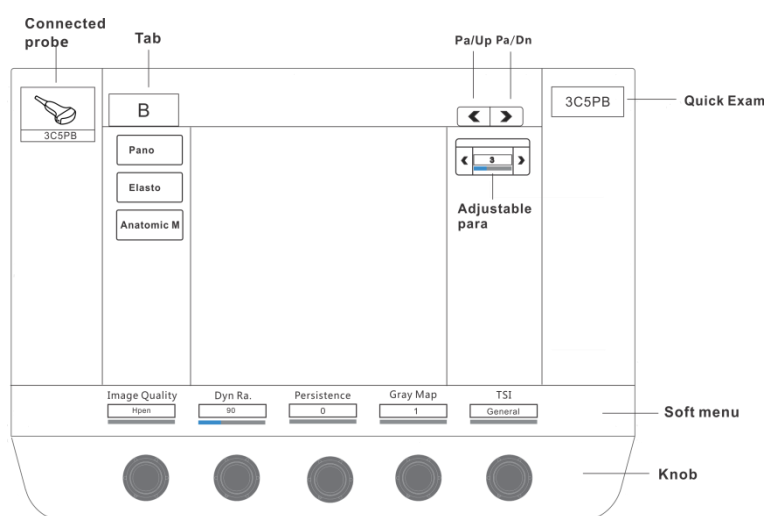


Figure 18 Touch Screen

Table 14 Touch Screen

Functional Area	Description
Connected probe	Display connected probe for quick switch.
Tab	Tap the corresponding tab on the touch screen can easily switch the corresponding screen or mode.
PaUp / PaDn	Tap to scroll up and down to display all items.
Adjustable Parameters	● If there is an adjustable parameter of menu item, tap [<] / [>] to adjust its value. ● If there is no adjustable parameters of menu item, tap the menu item to activate or enter the submenu; tap again to exit its function or submenu.
Quick Exam	Display quick exam mode for quick mode switch.
Soft Menu	Display the soft menu items of the Home screen synchronously.
Knob	Rotate the corresponding knob on the control panel to adjust the parameter.

Chapter 4 System Settings

4.1 Overview

This section details the access to configuration and service functions of the system. Customize your system to facilitate operation.

Item	Description
Enter the Preset screen	Press the <Setup> to enter the Preset screen.
Tab	Move the cursor over the tab and press the [Set] button to enter the corresponding setting screens.
Select an Item	Move the cursor over a setting item; press the [Set] button to select the item.
Text Box	Select the text box, enter text and numbers directly.
Drop-Down Box	Click the drop-down box to display all the sub-options under the current option.
Check box	Check the check box to activate corresponding option.
Save	Click to save current settings and return to the Home screen.
Cancel	Click to cancel all modifications and return to the Home screen.
Exit the Preset screen	In the Preset screen, press <Setup> again or click [Cancel] to cancel all modification and exit the Preset screen. In the Preset screen, click [Save] to save all modification and exit the Preset screen.

4.2 System Preset

4.2.1 Region

The Region tab is the default page of the Preset screen.

Open the Region tab via **[Preset]** (press **<Setup>**) → **[System Preset]** → **[Region]**. This tab is access to related information settings, such as hospital information, system language, and system time.

Figure 19 System Preset-Region

Table 15 System Preset-Region

Item		Description
Hospital Info	Name	Hospital Name.
	Address	Hospital Address.
	Telephone	Hospital telephone.
	Fax	Hospital Fax.
	Upload hospital logo	Click [Upload] , a dialog box pops up. Select the picture you want to upload, and click [OK] . After the upload is completed, the logo is displayed in the Logo area. This logo will be displayed in the Report review screen.
Language & Time	Languages	Set the system language.
	Date & Time	Set the current date and time of the system. Enter the date in the date and time bar, or select the date through the calendar. Delete the original value, and enter the correct value.
	Current Time	Set the current time of the system. Delete the original value, and enter the new value.
	Keyboard Layout	Set the keyboard layout.
	Time Zone	Set the time zone of the system.
	Date Format	Set the date format.
	Time Format	Set the time format of the system.

Item		Description
	Current Time	Set the current time of the system. Position the cursor behind the hour, minute, and second values in sequence. Delete the original value, and enter the new value.
	Sync	Synchronize system time to the system hardware time.

4.2.2 General

Open the General tab via **[Preset]** (press <Setup>) → **[System Preset]** → **[General]**.

This tab is access to settings of homescreen animal information (type, name, height unit, etc.), status after exam ends, system screen saver, and system time.

Figure 20 System Preset-General

Table 16 System Preset-General

Item		Description
Animal Info	Display Item	Set whether to display animal name, DOB (Date of Birth), gender, age, hospital, animal ID and operator information in the Home screen.
	Height and Weight Units	Set the Height and Weight units of animal.
	Body Surface Area Formula (BSA)	Set BSA formula.
Exam Settings	Status after exam ends	Set the status after exam ends.
	Send exam to DICOM after exam ends	Set whether to send the animal data automatically to the DICOM server for storage after exam ends.
System Screensaver	Screen Saver	Enable/disable the screen saver and set the waiting time before entering the screen saver state.

Item		Description
	Show login box when exiting screensaver	Set whether to show the login box when exiting the screen saver.
	Restore	Restore to the default screen saver.
	Select Picture	Select a picture as the screen saver.
	Preview	Preview the screen saver picture.
System Time	Display System Time	Set whether to display system time.

4.2.3 Image

Open the Image tab via **[Preset]** (press **<Setup>**) → **[System Preset]** → **[Image]**. This tab is access to related settings on save, output, display, and freeze for images and cines.

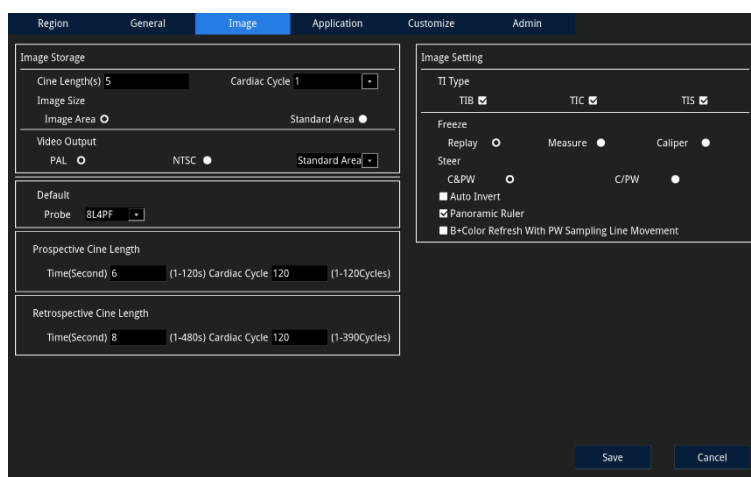


Figure 21 System Preset-Image

Table 17 System Preset-Image

Item		Description
Image Storage	Cine Length	Set the cine length.
	Cardiac Cycle	Set the cardiac cycle.
	Image Size	Set the save area of images. Image Area: image and image parameters Standard Area: image, image parameters, and information at the top of the Home screen
	Video Output	Set the format of video output / S-video output.
Prospective Cine Length		Set the cine length for prospective live capture and

Item		Description
		cardiac cycle.
Retrospective Cine Length		Set the cine length for retrospective live capture and cardiac cycle.
Default Image Settings	Probe	Set default probe.
	TI Type	Set whether to display the bone thermal index of bone (TIB), the thermal index of cranial (TIC) or thermal index of soft tissue (TIS) in the image area.
	Freeze	Set status after freeze.
	Zoom Type	Set the magnification type.
	Steer	Set whether to steer the sampling frame of the Color mode and the sampling line of the PW mode together under B + Color + PW mode.
	Auto Invert	Set whether the spectrum automatically inverts accordingly when the sampling line and the sampling frame are steered.
	Horizontal Ruler	Set whether to display horizontal imaging ruler.
	Center Line	Set whether to display center line.
	Panoramic Ruler	Set whether to display panoramic imaging ruler.
	B+Color Refresh with PW Sampling Line Movement	Set whether to activate B+Color live image when moving PW sampling line and freeze the B+Color image when stopping moving PW sampling line.

4.2.4 Application

Open the application tab via **[Preset]** (press **<Setup>**) → **[System Preset]** → **[Application]**. This tab is access to related setting of measurement and annotation.

The screenshot shows the 'Application' tab of the 'System Preset-Application' dialog. It is divided into two main sections: 'Measuring Cursor' and 'Annotation'.

Measuring Cursor Section:

- Type:** Radio buttons for Number, Symbol, and Small.
- Size:** Radio buttons for Large, Medium, and Small.
- Color (active):** Radio buttons for Green, Yellow, Red, and White.
- Color (inactive):** Radio buttons for Green, Yellow, Red, and White.
- Result Size:** Radio buttons for Super Large, Large, Medium, and Small.
- Cardiac Cycle:** A dropdown menu currently set to '2'.
- Delete measurement results when deleting calipers:** A checked checkbox.

Annotation Section:

- Font Size:** Radio buttons for Large, Medium, and Small.
- Arrow Size:** Radio buttons for Large, Medium, and Small.
- Automatically clear comments when unfreeze the image or switch the probe/exam mode:** A checked checkbox.
- Automatically clear the body mark when unfreeze the image:** An unchecked checkbox.

At the bottom right, there are 'Save' and 'Cancel' buttons.

Figure 22 System Preset-Application

Table 18 System Preset-Application

Item		Description
Measuring Cursor	Type	Set the cursor type.
	Size	Set the cursor size.
	Color (active)	Set the color of cursor and measurement results of activated state.
	Color (Inactive)	Set the color of cursor and measurement results of not-activated state.
	Result Size	Set the font size for measuring result.
	Cardiac Cycle	Set the number of cardiac cycles when taking heart rate measurement.
	Delete measurement results when deleting calipers	Set whether to clear the measurement results in the result window when deleting the calipers.
Annotation	Font Size	Set the font size for text annotation or comments.
	Arrow Size	Set the arrow size for arrow annotation.
	Automatically clear comments when unfreeze the image or switch the probe/exam mode.	Set whether to clear all comments or annotations on the image automatically when unfreezing the image, switching the probe, or switching the exam mode.
	Automatically clear the body mark when unfreeze the image	Set whether to clear the body mark automatically when unfreezing the image.

4.2.5 Customize

Open the Customize tab via **[Preset]** (press <Setup>) → **[System Preset]** → **[Customize]**. This tab is access to function definition for user-defined buttons and foot switch.

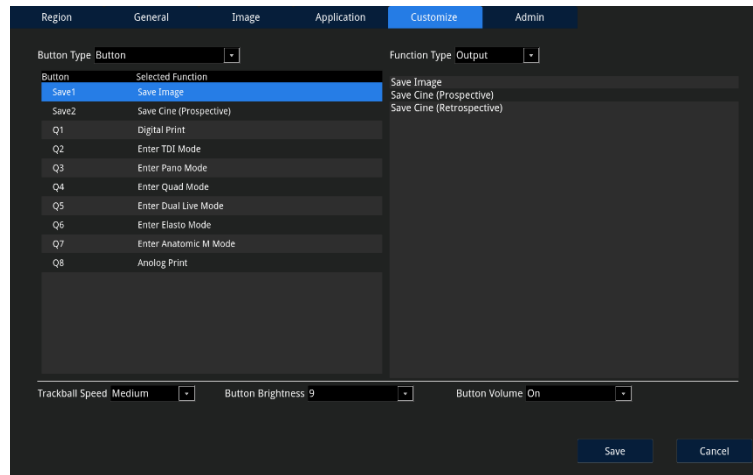


Figure 23 System Preset-Customize

Table 19 System Preset-Customize

Item	Description
Button Type	Select the button type you want to set.
Function Type	Select the function assigned by the button and the function list displays below.
Trackball Speed	Set the speed of trackball.
Button Brightness	Set the button brightness level.
Button Volume	Turn on/off the button volume function.

To customize user-defined button/foot switch, perform the following steps:

1. Click **[Button Type]** drop-down box and select button type.
2. Select a button you want to customize by pressing the **[Set]** button.
3. Click the **[Function type]** drop-down box to display all definable functions.
4. Double click a definable function to assign the function to the desired button.
5. Click the **[Save]** to save modifications and return to the Home screen.

4.2.6 Admin

The system supports three types of users: the administrator, operator and emergency user.

Icon	User	Permission
	Administrator	Access to all animal data in the system and be able to add users, delete users, import data, export data, delete data, edit data, store data, upgrade software / firmware, etc.
	Operator	Access to all animal data in the system and be able to import data, export data, delete data, edit data, and store data.
	Emergency user	Access to view and store animal data only. Data exporting, deleting and edition are not allowed.

4.2.6.1 Access Setting

Open the Permission tab via **[Preset]** (press **<Setup>**) → **[System Preset]** → **[Admin]**.

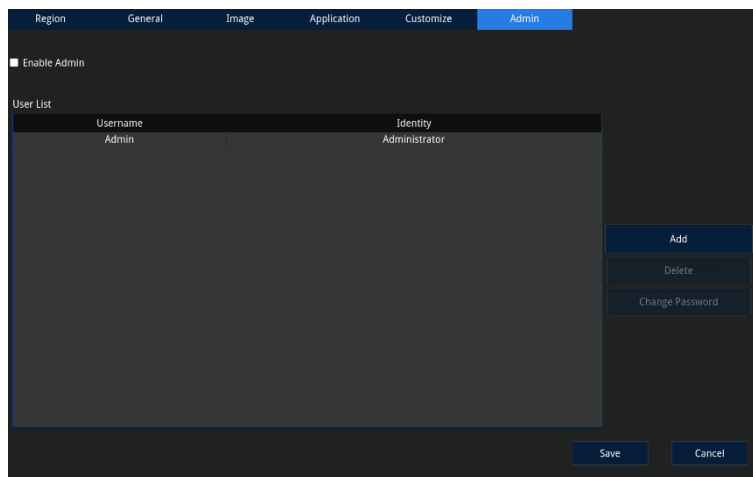


Figure 24 System Preset-Admin

Table 20 System Preset-Admin

Item	Description
Enable Admin	After enabling admin, login is required when exporting data, backing up data, deleting data, etc. Admin is not enabled by default.
Add	To add a new user: 1) Click [Add] to pop up the Add New User dialog box. 2) Enter a new user name, enter password, confirm the password, select a new user type, and click [OK] to complete adding a new user.
Delete	To delete an existed user: ● Select the target user in the user list and click [Delete].

Item	Description
Change Password	To modify the password of current user: 1) Select the target user in the user list and click [Change Password], a dialog box pops up. 2) Enter the new password, confirm the new password and click [OK] to complete the password modification.


NOTE: Only administrators can enable/disable admin and add/delete users.

4.2.6.2 System Login

When admin is enabled, you can access the data in the system only after login.

To log on the system:

1. The system pops up the login dialog box as shown below.

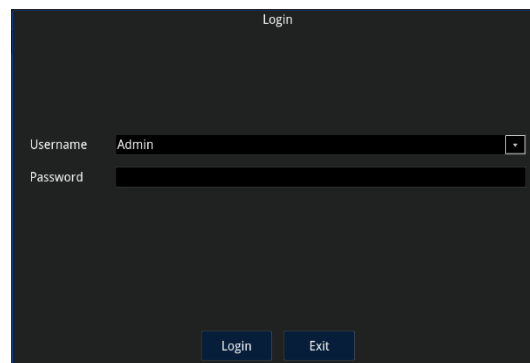


2. Click **[Username]** drop-down box to select the user name.
3. Enter correct password and click **[Login]**.

4.2.6.3 Change User

To change user:

1. Click the user icon “⌘” to pop up the dialog box as shown below.

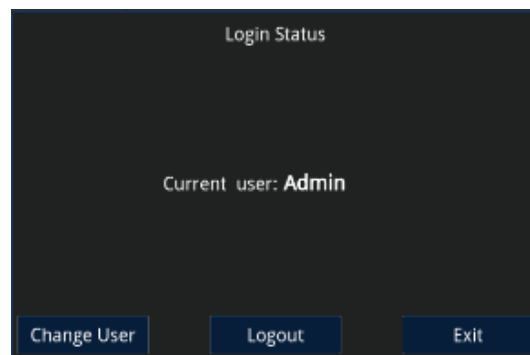


2. Click **[Change User]**, the login dialog box pops up.
3. Select desired user name and enter the password and then click **[Login]**.

4.2.6.4 System Logout

To log out the system:

1. Click the user icon “” to pop up the dialog box as shown below.

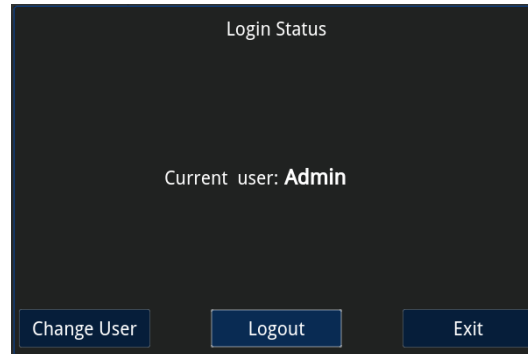

2. Click **[Logout]**.

4.3 Exam Preset

Enter the Exam Preset screen by clicking **[Exam Preset]** in Setup screen.

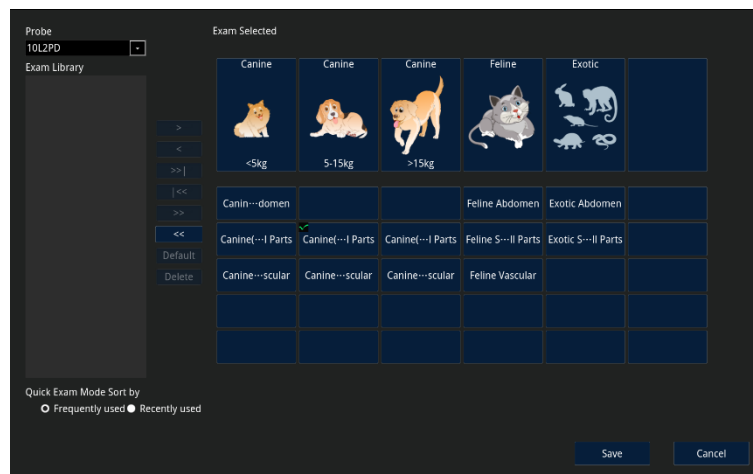


Figure 25 Exam Preset

Table 21 Exam Preset

Item	Description
Probe	Select a probe.
Exam Library	Display all available exam modes for current probe.
Exam Selected	Display all selected exam modes for current probe.
[<] / [>]	Add / Remove selected exam modes of current probe.
[<<] / [>>]	Add / Remove all exam modes of current probe (except for the default

Item	Description
	exam mode).
[<<] / [>>]	Add / Remove all exam modes of current animal (expect for the default exam mode).
Default	Set the selected exam mode as default for the current probe. Default exam mode is marked with a “√”.
Delete	Delete User-defined exam mode.
Quick Exam Mode Sort by	Set quick exam mode displaying order: either display the user's most frequently used, or most recently used exam modes on the touch screen (up to 7 can be displayed).

4.3.1 Add Exam Mode

To add an exam mode, perform the following steps:

1. Click the **[Probe]** drop-down box to select the probe type.
2. Select the desired exam mode list from the Exam Library.
3. Click the blank box of the Exam Selected area to determine the location to add exam mode.

If you do not assign a location, the system defaults to add an exam mode to the blank box in the order of top-down, left-to-right.
4. Click the **[>]** to add the selected exam mode to the Exam Selected area.

Or click the **[>>]** to add all exam modes from the Exam Library to the Exam Selected area.
5. Click **[Save]** to complete setting.

4.3.2 Remove Exam Mode

To remove exam mode:

1. Click the **[Probe]** drop-down box to select the probe type.
2. Select an exam mode you want to remove from the Exam Selected area.
3. Click **[<]** to remove the selected exam mode.

Or click **[<<]** to remove all exam modes listed in the Exam Selected area (expect for the default exam mode).
4. Click **[Save]** to complete setting.

4.3.3 Create/Delete User-defined Exam Mode

To create a user-defined exam mode:

1. Press the **<QSave>** on the keyboard to open the QSave dialogue box.
2. Rename and select data source and then click **[Create]** to create a user-defined exam mode.

To delete a user-defined exam mode:

1. Select the user-defined exam mode you want to delete in the Exam Preset screen.
2. Remove the desired exam mode to the Exam library and click **[Delete]** to delete a user-defined exam mode.

4.3.4 Adjust Exam Mode Display Position

The position of the exam mode displayed in the Exam Selected/ QuickExam selected area will be synchronously displayed on the touch screen. You can adjust the display position of the exam mode to facilitate operation by following methods:

➤ **Method 1**

Select an exam mode to move and click on a blank box.

The selected exam mode will be moved to the blank box position.

➤ **Method 2**

Click two exam modes to exchange the positions of these two exam modes.

4.4 Measure Preset

Enter the Measure Preset screen by clicking **[Measurement Preset]** in the Preset Screen. The Measure Preset is access to related settings for general measure items, application measure items and report templates.

4.4.1 General Measurement Preset

To preset the general measurement:

1. Click **[Caliper]** tab to enter the general measurement preset page. The left column lists available measurement items while the right column lists selected measurement items.
2. Click **[2D]**, **[M]**, or **[Doppler]** tab to set measurement items under corresponding imaging mode.
3. Click **[Measurement Package]** drop-down box to select an exam mode.
4. Set measurement item.

Operation	Description
Add Measurement Item	1) Select the item(s) you want to add from the left column. 2) Click [>] to add the selected items of the left column to the right column. Or Click [>>] to add all items of the left column to the right column.
Remove measurement Items	1) Select the item(s) you want to add from the left column. 2) Click [<] to remove the selected items from the right column to the left column. Or Click [<<] to remove all items from the right column to the left column.
Adjust measurement item position	Select a selected measurement item and click [Up] / [Down] to adjust the position of the measurement items.
Set default measurement item	Select a selected measurement item and click [Default] to set the measurement item as default. Default measurement item is marked with a "√".
Set Measurement Item Property	Select a selected measurement item, click [Property] to open the properties dialog box. Check the items to display in the result window or set the measurement item properties.
Status after completing current measurement.	Click on the [Measurement Sequence] drop-down box to set the status after completing current measurement. ● None: No measurement item is activated after completing the current measurement. ● Repeat: Activate the current measurement item again after completing the current measurement. ● Next: Activate the next current measurement item after completing the current measurement.

5. Click **[Save]** to save current settings and return to the Home screen.

4.4.2 Application Measurement Preset

To preset application measurement item:

1. Click **[Measure]** tab to enter the application measurement preset page.
The left column lists available measurement items while the right column lists selected measurement items.
2. Click **[2D]**, **[M]**, or **[Doppler]** tab to set measurement items under corresponding imaging mode.
3. Click **[Measurement Package]** drop-down box to select an exam mode.
4. Set measurement item.

Operation	Description
Add Measurement Item	1) Select the item(s) you want to add from the left column. 2) Click [>] to add the selected item of the left column to the right column. Or click [>>] to add all items of the left column to the right column.
Remove Measurement Item	1) Select the item(s) you want to remove from the right column. 2) Click [<] to remove the selected item from the right column to the left column. Or click [<<] to remove all items from the right column to the left column.
New	Open the Customize Wizard dialog box.
Delete	Remove a customized measurement item.
Advanced	Open the Advanced Setting dialog box.
Adjust Measurement Item Position	Select a selected measurement item and click [Up] / [Down] to adjust the position of the measurement items.
Set Default Measurement Item	Select a selected measurement item and click [Default] to set the measurement item as default. Default measurement item is marked with a “√”.
Set Measurement Item Property	Select a selected measurement item, click [Property] to open the properties dialog box. Check the items to display in the result window or set the measurement item properties.
Status after completing current measurement.	Click [Measurement Sequence] drop-down box to set the status after completing current measurement. ● None: No measurement item is activated after completing the current measurement. ● Repeat: Activate the current measurement item again after completing the current measurement. ● Next: Activate the next current measurement item after completing the current measurement.

5. Click **[Save]** to save current settings and return to the Home screen.

4.4.2.1 Customize Application Measurement / Calculation Item

To customize application measurement / calculation item:

1. Click **[New]** to open the Customize Wizard dialog box.

2. Enter an item name, select item type, and click on **[Next]**.
3. Set measurement item properties.
4. Click **[Complete]** to save the customized measurement/calculation item settings and close the Customize Wizard dialog box. The customized measurement / calculations items are displayed at the bottom of the list of available measurement items on the left.

4.4.2.2 New Study

1. Select the measurement package you want to add a new study.
2. Click **[New Study]** to open new study dialog box.
3. Enter the name of the new study and click **[OK]**. The new study is displayed at the bottom of the list on the right.

4.4.2.3 Edit Measurement Package

To edit measurement package:

1. Click **[2D]**, **[M]** or **[Doppler]** tab to set the imaging mode of the measurement package.
2. Click **[Advanced]** to enter the New Measurement Package screen. Available packages are listed in the left column while the selected packages are listed in the right column.
3. Edit Measurement package. You can add, remove, adjust the measurement package order, and set the default measurement package.

Operation	Description
Add Measurement Package	1) Select the package(s) you want to add from the left column. 2) Click [>] to add the selected package from the left column to the right column. Or click [>>] to add all packages from the left column to the right column. 3) The measurement package can be activated by rotating the knob under the [Exam] button of the touch screen.
Remove Measurement Package	1) Select the package(s) you want to remove from the right column. 2) Click [<] to remove the selected package from the right column to the left column. Or click [<<] to remove all packages from the right column to the left column.
New	Open the input dialog box and enter the measurement package name.
Delete	Remove a customized measurement package.
Adjust	Select a selected measurement package and click [Up] / [Down] to adjust

Measurement Package Position	the measurement package position.
Set Default Measurement Package	Select a selected measurement package and click [Default] to set the measurement package as default. Default measurement package is marked with a “√”.

- Click **[OK]** to exit the New Measurement Package screen and the current measurement package will be replaced by the new default measurement package.

4.4.3 Report Template

Click **[Report]** tab to enter the Report Preset screen. This tab is access to relevant settings of report template.

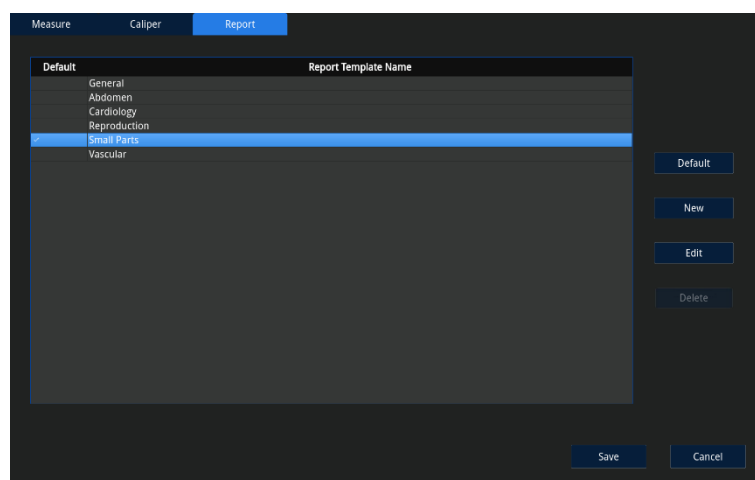


Figure 26 Measure Preset- Report

4.4.3.1 Default Report Template

Select a report template in the report template list and click **[Default]** to set the template as default.

Default report template is marked with a “√”.

4.4.3.2 New Report Template

- Click **[New]** to pop up new report template dialog box.
- Enter the name of the report.
- Set the measurement results displayed in the report template.

Operation	Description
Add measurement result in the report	- Click [Optional Items] drop-down box, select the exam mode, and select the corresponding item type in the right drop-down box. - Select a result item from the left column.

Operation	Description
	3) Click [>] to add the measurement result item to the report; Or click [>>] to add all measurement result items to the report.
Remove measurement result from the report	1) Select a result item from the right column. 2) Click [<] to remove the measurement result item of the report; Or Click [<<] to remove all the measurement result items from the right column to the left column.
Adjust measurement result position	Select a measurement result item in the right column, and click [Up] / [Down] to adjust the position of measurement results displayed in the report.

4. Click **[OK]** to exit the report template screen, and the new report template is displayed in the report template list.

4.4.3.3 Edit Report Template

1. Select a report template in the report template list.
2. Click **[Edit]** to enter the report template edit screen.
3. Complete relevant settings as needed.
4. Click **[OK]** to save modifications and exit the report template edit screen.

4.4.3.4 Delete Report Template

Select a report template in the report template list and click **[Delete]** to delete the template.

4.5 zWorkflow Preset

Users can use the auto workflow template for an automatic scan. The auto workflow function will help to reduce unnecessary operation and improve the exam efficiency.

4.5.1 Workflow Protocol

A workflow protocol should be set before using the auto workflow function.

In the Preset screen, select **[zWorkflow Preset]** to enter the zWorkflow setting screen.

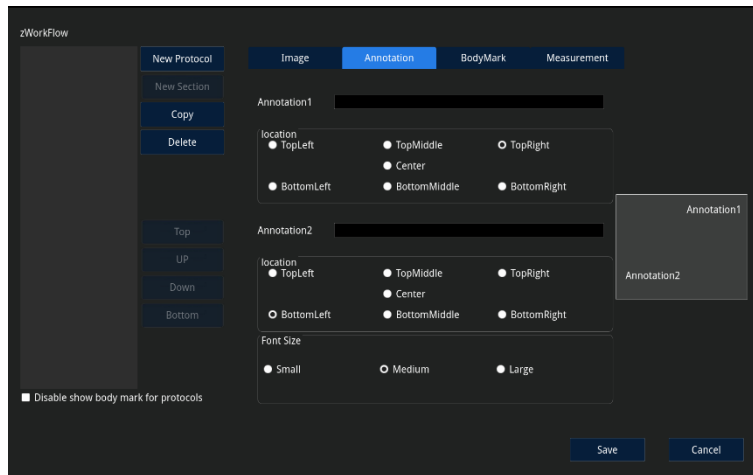


Figure 27 zWorkflow

Table 22 zWorkflow

Item	Description
Protocol List	List all stored protocols.
New Protocol	Create a new user-defined protocol.
New Section	Add a new view for selected protocol.
Copy	Copy a protocol.
Delete	Delete a protocol.
Top	Move the selected protocol to the top of the list.
Up	Move the selected protocol up.
Down	Move the selected protocol down.
Bottom	Move the selected protocol to the bottom.

4.5.2 New Protocol

To create a new protocol, please perform the following steps:

1. In ZWorkflow preset screen, click **[New Protocol]**, enter protocol name to create a new protocol.
2. Select protocol type and application.
3. Click **[New Section]** to enter the section name, and perform image, comments, body mark, measurement settings as needed.
4. Use the check box for auto OB measurement and body mark display settings.
5. Click **[Save]** to complete the setting and exit.

4.5.3 Basic zWorkflow Procedures

1. Tap **[ZWork]** on the touchscreen to activate zWorkflow function.

2. Enter and save animal's information.
3. Select desired protocol from the touchscreen.
4. Complete the scanning and saving of all sections according to the selected protocol, and complete the exam.
5. Perform measuring, add annotations or body mark as needed.
6. Tap **[ZWork]** again to exit zWorkflow function.

4.5.4 Section Operation

In zWorkflow status, you can perform section selection, operation, repetition, replacement and deletion by the touch screen.

➤ **Selection**

Tap **[Previous]** / **[Next]** to select the section to be scanned, the current section is around by a green frame.

➤ **Operation**

In the current active view, you can perform image scanning, measurements, adding comments and body mark and etc.

➤ **Repetition**

Tap **[Repeat]** to insert another template of the current view, then you can perform an extra examination.

➤ **Redo**

Tap **[previous]/[Next]** to select the section to be redone, and then tap **[Redo]** to redo the selected section.

➤ **View Deletion**

Tap **[previous]/[Next]** to select the section to be deleted, and then tap **[Delete]** to delete the selected section.

➤ **Undone Section**

Tap **[Undone Section]** to check and select undone section quickly.

4.6 Network Preset

Network preset includes local and DICOM service-related network settings.

This section only introduces the local network setting. For details about the DICOM service-related network settings, refer to “Chapter 11 DICOM”.

In the Preset screen, select **[Network Preset]** → **[Local TCP/IP]** to enter the local network setting screen. This screen is access to local network and LAN settings.

Figure 28 Network Preset- local TCP/ IP

Table 23 Network Preset- local TCP/ IP

Item	Description	
Wired Network	Network Acquiring	Select network acquiring method.
	IP Address	The IP address of system should be in the same network segment as the IP address of the server.
	Subnet Mask	Enter the subnet mask address of the system to set different network segments.
	Gateway	Enter the gateway address of the system.
	Apply	Click to make the modifications in this network property effective.
Wireless Network (Reserved function)	Auto Connection	Turn on/off the auto connection function.
	Refresh	Click to refresh the wireless network.

NOTE: IP address should not be occupied by other device in the LAN. Malfunction of DICOM will result.

4.7 Print Preset

In the Preset screen, select **[Print Preset]** to enter the print preset screen. This screen is access to printing settings.

To add a printer, refer to “3.10.2 Connect Printer” for details.

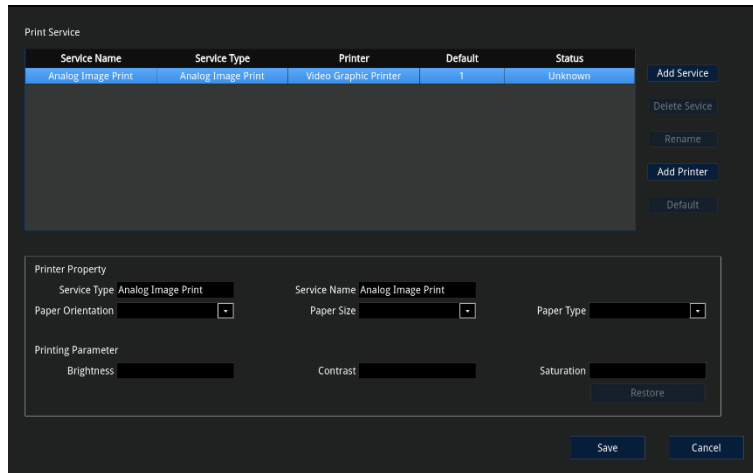


Figure 29 Print Preset

Table 24 Print Preset

Item		Description
Print Service	Add Service	Click to open the add service dialog box.
	Delete Service	Click to remove the selected service.
	Rename	Click to rename the selected service.
	Add Printer	Select printer driver and performs related settings.
	Default	Click to set the selected service as default.
Printer Property	Service Type	Display service type of the printer.
	Service Name	Display service name of the printer
	Paper Orientation	Set the paper orientation for printing.
	Paper Size	Set the paper size for printing.
	Paper Type	Set the paper type for printing.
Printing Parameter	Brightness	Set the brightness for printing.
	Contrast	Set the contrast for printing.
	Saturation	Set the saturation for printing.
	Restore	Restore default parameter setting for printing.

4.8 Maintenance Preset

In the Preset screen, select **[About & Maintenance]** to enter the Maintenance Preset screen.

This screen is access to system information, detailed information, option and other. You can view system information and configure options and other settings.

4.8.1 System Information

Select **[About & Maintenance]** → **[System Info]** to enter the System Information screen, where you can view the release version information of the system.

4.8.2 Detailed Information

Select **[About & Maintenance]** → **[Detailed Info]** to enter the Detailed Information screen, where you can view the detailed information of the system.

The displayed information varies depending on the configuration and version of the system.

4.8.3 Option

Select **[About & Maintenance]** → **[Option]** to enter the Option screen. This screen lists all the available options and their installation status. You can also view the machine code in this screen and contact the dealer to complete the whole machine authorization.

4.8.4 Other

Select **[About & Maintenance]** → **[Other]** to enter the Other screen.

This screen is access to import / export for preset data and exam mode, restore factory defaults and upgrade.

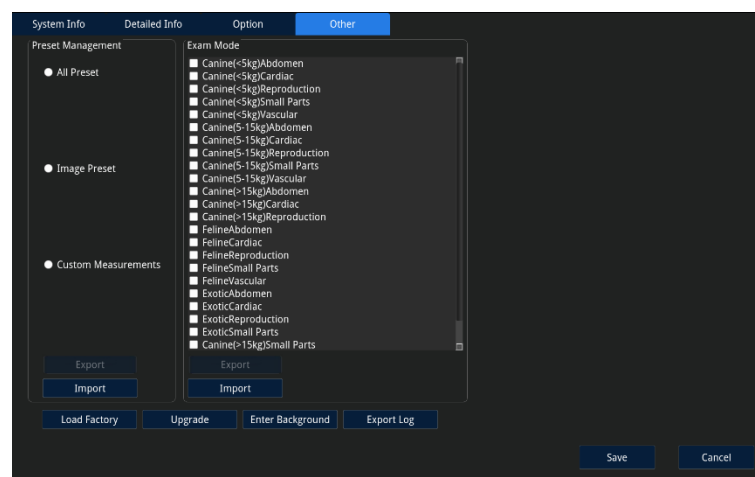


Figure 30 About & Maintenance- Other

Table 25 About & Maintenance- Other

Item		Description
Preset Management	All Preset	Select management preset data to all preset.
	Image Preset	Select management preset data to image preset.

Item		Description
	Custom Measurements	Select all management preset data to customized measurement preset.
	Export	Export selected preset data.
	Import	Import preset data to the system.
Exam Mode	Export	Export selected exam mode.
	Import	Import exam mode to the system.
Load Factory		Restore all settings to factory defaults.
Upgrade		Upgrade software versions.
Enter Background		Enter engineering mode. Only available to authorized personnel.
Export Log		Export the log. Only available to authorized personnel.

NOTE: DO NOT remove the USB device or shut down the system during software upgrade.

Chapter 5 Preparing an Exam

5.1 Animal Information

Although the system supports exam without entering animal information, to avoid data chaos, it is recommended to enter animal information before performing an exam for better animal data management.

For archived animals, you can obtain animal information via the local and DICOM servers.

5.1.1 New Animal

Enter the animal information prior to the exam for the first time.

To start a new animal, perform the following steps:

1. Press **[Patient]** button on the control panel to enter the Animal Information screen.

Basic Info

Animal Name: _____ Animal ID: 20231110-103039-8278 Animal No.: _____

Gender: _____ Age: _____ Year: _____ DOB: _____ [Worklist]

Host: _____ Animals: _____ Canine(<Skg): _____ Sterilization: _____

Abdomen Reproduction Cardiology Vascular Small Parts

LMP: _____ [Calendar]

Gravida: _____ Para: _____

Ectopic: _____ Abortion: _____

Gestations 1: _____

Exam Description: _____ Accession: _____ Comment: _____

Symptom: _____ Clinician: _____

Past History: _____ Diagnostician: _____

Charge Code: _____ Operator: _____

Charge Description: _____

[New Animal] [New Exam] [End Exam] [Cancel Exam] [Save] [Cancel]

Figure 31 Animal Information Screen

Table 26 Animal Information Screen

Item	Description
Worklist	Click to enter the Worklist screen.
New Animal	Click to erase all animal data and create a new animal record by entering new animal information.
New Exam	Click to end current exam and create a new exam for current animal.
End Exam	Click to end the current exam.
Cancel Exam	Click to cancel the current exam. Canceled exam cannot be restored.
Save	Click to save animal information and return to the home screen.
Cancel	Click to cancel animal information input and return to the home screen.

2. Move the cursor to the desired text box and enter the animal basic information.

Exam Information	Description
Animal Name	Enter animal name.
Animal ID	The system generates the animal ID automatically. To enter the animal ID manually, please delete the default animal ID first and then enter the new ID.
Animal No.	The system auto-synchronizes the serial number of the same animal in the worklist.
Gender	Click drop-down box to select animal gender.
Age	Enter the date of birth; the system will automatically calculate the animal's age. Otherwise, manual input is required.
DOB	Enter directly in the text box, or click the drop-down box to select the animal's date of birth in the calendar.
Host	Enter host name.
Animal Type	Select animal type.
Sterilization	Select sterilization status.

NOTE: Use keyboard for information entry. Press <Ctrl> + <Space> to switch input method between Chinese and English.

3. Click the corresponding tab to select the appropriate exam type, and enter the animal's exam information.

- Available exam types are: ABD (Abdomen), REP (Reproduction), CARD (Cardiology), VAS (Vascular), and SMP (Small Parts).
- Exam-specific information is required for different exam types.

Exam Type	Exam Information	Description
Abdomen	Height	/
	Weight	/
	BSA (Body Surface Area)	After entering the weight, the system calculates the BSA according to the formula selected by the user. To set the BSA formula, refer to "4.2.2 General" for details.
Reproduction	Calculation Index	LMP: enter the last menstrual period.

Exam Type	Exam Information	Description
	Gestations	Select fetus number. The system supports up to 15 fetus measurements.
	Gravida	Times of pregnancy.
	Para	Times of delivery.
	Ectopic	Times of abnormal pregnancy. (E.g. Ectopic pregnancy)
	Abortion	Times of abortion.
Cardiology	Height	/
	Weight	/
	BSA (Body surface area)	After entering the weight, the system calculates the BSA according to the formula selected by the user.
	HR	Heart rate of the animal.
	RA Press	Right atrium pressure of the animal.
	BP	Blood pressure of the animal.
Vascular	Height	/
	Weight	/
	BP (L)	Left blood pressure of the animal.
	BP (R)	Right blood pressure of the animal.
Small Parts	/	/

4. Enter operation information.

Operation Information	Description
Exam Description	Briefly describe the exam.
Symptom	Explain the reasons for performing ultrasound exam.
Past History	Enter the previous medical history of the animal.
Charge Code	Enter the charge code.
Charge Description	Briefly describe the charge information.
Accession	Enter the accession number.

Operation Information	Description
Clinician	Enter the name of the clinician.
Diagnostician	Enter the name of the diagnostician who is responsible for the exam.
Operator	Enter the name of the operator.
Comment	Enter supplementary exam information.

5. Click **[Save]** to save the animal information and return to the Home screen.

- NOTE:**
- In case of emergency, you can perform an exam directly without animal information entry.
 - When an image or cine is frozen, the system automatically generates an animal ID.

5.1.2 Retrieve Animal Information (Station)

For animal information stored in the local hard disk, you can obtain animal information through the Station screen.

To retrieve animal information, perform the following steps:

1. Press **<Station>** key to enter the Station screen.

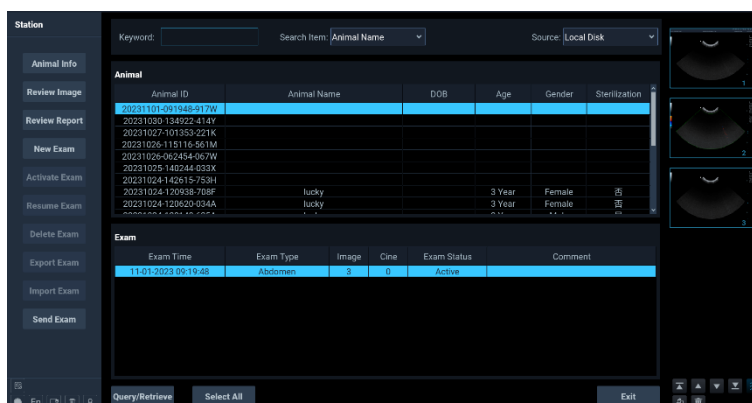


Figure 32 Station Screen

2. Click **[Source]** drop-down box to select the storage location of the desired animal information.
3. Search the desired animal.

Item	Description
Keyword	Enter the keyword for the search item. The animal list shows the animals who meet the requirements, the exam list shows all the exams under the selected animals, and the system defaults to select the first animal in the animal list.
Search Item	Click [Search Item] drop-down box to select a search item among animal

	name, animal ID, DOB, and exam date.
--	--------------------------------------

4. Select the desired animal and press the **[Set]** button to open the operation menu.

Item	Description
Animal Info	Click to enter the animal information screen, and view the selected animal information.
Review Image	Click to enter the review screen, and review the images of the selected exam.
Review Report	Click to enter the report screen and review the selected report. (unavailable for canceled exams)
New Exam	Click to create a new exam for the selected animal.
Activate Exam	Click to continue an exam that ends within 24 hours.
Resume Exam	Click to continue an exam that was interrupted within 24 hours.
Delete Exam	Click to delete the selected exam.
Export Exam	Click to export the selected exam to the storage media supported by the system.
Import Exam	Click to import animal information from other media to the system.
Send Exam	Click to send the selected exam to the external storage media, DICOM server or printer.
Query / Retrieve	Click to view animal information stored on the DICOM server.
Select All Exams	Click to select all animals and exams for batch operations.
Exit	Click to exit Station screen and return to the home screen.
^ / ^	Click to go to the previous/next page.
⏮ / ⏭	Click to go to the first/last page.

5.1.3 Retrieve Animal Information (DICOM)

After the system is connected to the DICOM server and the worklist server is set up (refer to “11.1.2.3 Worklist” for more information). You can remotely query or import animal information via the worklist server. Refer to “11.2.3 DICOM Worklist” for details.

5.2 Select Probe and Exam Mode

NOTE: ● If the exam mode is switched during the measurement, all general measurement data will be cleared while the application measurement

data will be saved in the report.

- Freeze the image or shut down the system power before connecting or removing the probe. Otherwise, system and probe damage may result.
- After replacing the probe, please switch over to the new probe on the Probe / Exam mode screen.

To select probe / exam mode, perform the following steps:

1. Connect the probes to the probe receptacle. (Refer to “3.6 Connect / Remove the Probe” for details).
2. Press **[Probe]** button on the control panel to enter the Probe / Exam mode screen. Connected probes and corresponding exam modes are displayed on the touch screen.

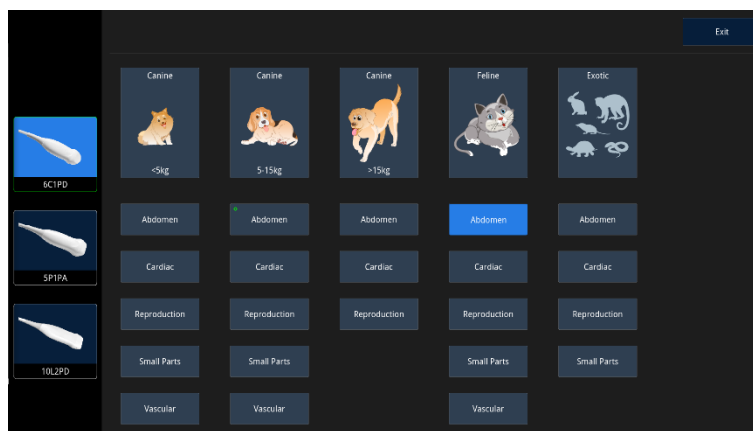


Figure 33 Probe/Exam Mode Screen

3. Click the probe icon to select an appropriate probe.
4. Select the desired exam mode and the system enters the corresponding exam mode.
5. Click **[Exit]** or press **[Probe]** button again to exit the Probe / Exam mode screen.

5.3 Select Imaging Mode

Select an appropriate imaging mode. Refer to “Chapter 6 Optimizing the Image” for more information of each imaging mode.

5.4 Resume/Activate Exam

5.4.1 Resume Exam

To resume an interrupted exam, perform the following steps:

1. Press **<Station>** key to enter the Station screen.
2. Select the desired animal and exam.

3. Click **[Resume Exam]** to load the animal basic information and measurement data to resume the previously interrupted exam.

NOTE: Only exams interrupted within 24 hours can be resumed.

5.4.2 Activate Exam

For animals that have completed the exam but need to be re-examined, perform the following steps:

1. Press **<Station>** key to enter the Station screen.
2. Select the desired animal and exam.
3. Click **[Activate Exam]** to load the animal basic information and measurement data to resume the previously completed exam.

NOTE: Only exams completed within 24 hours can be reactivated.

5.5 Cancel / End Exam

5.5.1 Cancel Exam

To cancel an exam, perform the following steps:

1. Press the **[Patient]** button on the control panel to enter the animal information screen.
2. Click **[Cancel Exam]** to pop up the Cancel exam dialog box.
3. Click **[OK]** to cancel the exam or **[Cancel]** to resume the current exam.

5.5.2 End Exam

To avoid data chaos between different animals and measurement items, end the current exam before proceeding to the next exam.

1. To end the current exam:
 - Press the **[EndExam]** button on the control panel.
 - Press the **[Patient]** button on the control panel to enter the animal information screen. Click **[New Animal]** or **[New Exam]** or **[End Exam]**.
2. The end exam dialog box pops up. Click **[OK]** to save the current animal data and exit the current exam.

Chapter 6 Optimizing the Image

6.1 Imaging Mode

The system offers a set of imaging modes to accommodate a variety of imaging applications. Special modes are also available for panoramic imaging, elastography, and TDI imaging.

The system supports following imaging modes:

Imaging Type	Imaging Mode
B	B-mode, 2B mode, 4B mode
M	M-mode, Anatomic M mode, Color M mode
Color	Color mode, PDI mode, DPDI mode
Doppler	CW mode, PW mode
Special	Panoramic imaging, Elastography, TDI imaging

6.2 Operation Interface

The operating interface of this system consists of a Home screen and a touch screen. The home screen utilizes the trackball, cursor, and keyboard in conjunction to perform operations. The touchscreen, on the other hand, involves using finger taps and knobs on the control panel to carry out corresponding operations. For details, please refer to “3.12 Screen” and each chapter.

6.3 B-mode

The B-mode imaging uses a multi-beam scanning method to form each scanning line into a 2D grayscale image, and displays the strength of the tissue echo signal by the intensity of the brightness.

B-mode imaging is the most basic imaging mode by displaying the anatomical structure of tissues and organs in real time.

B-mode can also be used together with other modes.

6.3.1 Basic Procedure of B-mode

To perform B-mode imaging, perform the following steps:

1. Start a new exam.

2. Select an appropriate probe and exam mode, the system enters B-mode by default or press the **[B]** knob on the control panel to enter B-mode.
3. Optimize the image. (Refer to “6.3.2 Image Optimization (B)” for details)

The parameter area provides real-time parameter information of the B mode. The meanings of each parameter are as follows:

Parameter	B (2D) Mode
F	Working Frequency (MHz)
D	Depth
G	Gain (dB)
FR	Frame Frequency
DR	Dynamic Range
ZClear	Image Enhancement

4. Perform measurements and calculations as needed.

6.3.2 Image Optimization (B)

The screen displays the relevant imaging parameters and image options.

You can optimize the B image by tapping the corresponding parameter on the touch screen or by rotating/pressing the corresponding knob on the control panel.

6.3.2.1 Gain

The gain is used to adjust the brightness of the B image. You can brighten the image and observe more echo signals by increasing the gain. However, with increased gain, more noise would be introduced.

Operation:

Rotate the **[B]** knob on the control panel to adjust the gain value.

6.3.2.2 TGC

The TGC controls compensation for signal attenuation as depth increases by varying the gain of the received signals at a specific depth.

Operation:

Move the eight TGC sliders on the control panel to adjust the brightness of the segmented image of the corresponding depth.

6.3.2.3 LGC

The LGC improves the lateral resolution of the image by adjusting the gain of the direction of the scanning line. The LGC curve is displayed above the image area when adjusting.

Operation:

- Click **[LGC]** on the touch screen to enter the adjustment interface, and the touch screen displays the 10-segment control slider.
- Move the corresponding slider to adjust the corresponding transverse segmentation image.

6.3.2.4 Depth

Depth controls the field of view. Increase the depth to look at a deeper or larger tissue structure, decrease the depth to look at tissue structures near the skin line. Increase the depth tends to decrease the frame rate.

Operation:

Toggle the **[Depth]** control on the control panel up and down to adjust the image depth.

NOTE: Adjustable range depends on the current probe. The actual depth is shown in mm in the image parameter area.

6.3.2.5 Steer

Steer control is used to deflect the direction of beam without moving the probe.

NOTE: Applicable to linear probes only.

Operation:

Rotate the **[Angle/Steer]** knob on the control panel to adjust the direction of the ultrasonic beam.

6.3.2.6 Auto-optimization

The system automatically optimizes image parameters based on the tissue characteristics of the current scan area.

When auto-optimization function is enabled, an "Auto" mark is displayed in the image parameter area.

Operation:

Press the **[Auto]** knob on the control panel to enable/disable auto optimization.

6.3.2.7 Image Quality

Adjust image quality by controlling the frequency. User selects the appropriate frequency type and frequency value based on the depth of scanning and tissue characteristics to achieve optimal imaging results.

The fundamental wave is marked with an "F" while the harmonic wave is marked with an "F H".

Operation:

1. Press the knob under **[Image Quality]** to switch between **[Fundamental Frequency]** and **[Harmonic Frequency]**.

2. Rotate the knob under **[Image Quality]** to select the frequency.

- Fundamental frequency options: Pen (Penetration priority), Gen (General imaging), Res (Resolution priority)
- Harmonic frequency options: HPen (Penetration priority), HGen (General imaging), HRes (Resolution priority), HPen-Gen (between Penetration and General)

NOTE: Adjustable range depends on the current probe.

6.3.2.8 Dynamic Range

Change the display range of the grayscale to adjust the contrast of the image.

Operation:

Rotate the knob under **[Dyn Ra.]** to adjust the dynamic range.

6.3.2.9 Persistence

Superimpose and average the images of adjacent frames to remove the noise and enhance the details. Low persistence can improve live images and is better for fast-moving organs, while high persistence can reduce noise and improve image clarity.

Operation:

Rotate the knob under **[Persistence]** to adjust the persistence value.

6.3.2.10 ZClear

Used to enhance image contrast, smooth images and reduce noise.

Operation:

Rotate the knob under **[ZClear]** to adjust the image enhancement.

6.3.2.11 Gray Map

Optimize the images by adjusting the black-white contrast of the image.

Operation:

Rotate the knob under **[Gray Map]** to adjust the grayscale.

6.3.2.12 Field of View

Change the scan range without moving the probe or ROI box.

You can get a wider scan range with a larger field of view (FOV). A larger FOV trends to decrease the frame rate.

Operation:

Tap [**<**] / [**>**] of **[Field of View]** on the touch screen to adjust the scan range.

6.3.2.13 Compound Imaging

Compound imaging is the process of merging frames of different steering angles into a single frame. This function is used to improve the spatial resolution and signal-to-noise

ratio of the image, making the image subtle and clean.

There are two types of compound imaging: SCI (Spatial Compound Imaging) and FCI (Frequency Compound Imaging).

SCI and FCI cannot be used simultaneously. When one of the compounds imaging type is activated, the other type will automatically turn off. Also, SCI may not be used in conjunction with Extended Filed-of-View (EFOV) and FCI may not be used in conjunction with harmonic imaging.

➤ **SCI (Spatial Compound Imaging)**

NOTE: SCI is not available for phased array probes.

Operation:

Tap [**<**] / [**>**] of [**SCI**] on the touch screen to adjust SCI levels.

➤ **FCI (Frequency Compound Imaging)**

FCI is only available for the fundamental frequency.

Operation:

Tap [**<**] / [**>**] of [**FCI**] on the touch screen to adjust FCI level.

6.3.2.14 Line Density

Line density determines the number of the ultrasonic scanning lines of a certain width or angle. The higher the line density, the higher the lateral resolution of the image and the lower the frame rate.

Operation:

Tap [**<**] / [**>**] of [**Line Density**] on the touch screen to adjust line density level.

6.3.2.15 Chroma

Replace grayscale distinction with color distinction to intuitively show grayscale level of the images. Chroma color is displayed on the grayscale bar.

Operation:

Tap [**<**] / [**>**] of [**Chroma**] on the touch screen to change the color.

6.3.2.16 EFOV (Extended filed-of-view)

When the extended imaging function is enabled, trapezoidal imaging (for linear array probes) or extended scanning angle (for convex array) will be displayed.

Operation:

Tap [**>**] on the touch screen to turn the page, and then tap [**<**] / [**>**] of [**EFOV**] to adjust the EFOV level.

6.3.2.17 TSI

Select the acoustic velocity according to the scanning parts to highlight the tissue texture.

Operation:

Tap [**>**] on touch screen to turn the page, and then tap [**<**] / [**>**] of [**TSI**] to select the tissue texture. Select [**Auto**] to set automated TSI.

6.3.2.18 Image Rotation

Change the orientation of the image display.

Operation:

- Tap [**>**] on the touch screen to turn on the page and then tap [**<**] / [**>**] of [**Rotation**] on the touch screen to change the image display.
- Rotation options: 0°, 90°, 180°, and 270°.

NOTE: “●” of the image corresponds to the orientation mark on the probe.

6.3.2.19 Focus Position/Number

Adjust the focus of the ultrasonic beam to increase the resolution of the particular area and focus the optimized image.

The focus symbol “◀” is displayed on the image depth scale.

➤ Adjust the focus position

Toggle the [**Focus**] control on the control panel up and down to adjust the focus position.

➤ Adjust the focus number

Tap [**>**] on touch screen to turn the page, and then tap [**<**] / [**>**] of [**Focus number**] to adjust the number of focus.

- NOTE:**
- Disable the SCI function before adjusting the focus number.
 - Phased array probe does not support adjusting the focus number.

6.3.2.20 Acoustic Power

Adjust the acoustic power of current selected probe in B-mode. Acoustic power value is displayed at the top of the screen.

Operation:

Tap [**>**] on touch screen to turn the page, and then tap [**<**] / [**>**] of [**A.Power**] to adjust the acoustic power.

6.3.2.21 Image Reverse

Reverse the image orientation horizontally or vertically for better observation.

Operation:

Tap [**UD Reverse**] or [**LR Reverse**] on the touch screen to turn on/off the image reverse function.

6.3.2.22 Dual Live

Display different image effects with two live images of one probe for better observation.

Operation:

Tap **[Dual Live]** on the touch screen to turn on/off the function.

A dual-split window displays on the screen and you can adjust the parameters of two B images via two tabs on the touch screen where shared and left image parameters displayed on **[B(L)]** tab while right image parameters displayed on **[B(R)]** tab.

6.3.2.23 Horizontal Scale

Display or hide the horizontal scale.

Operation:

Tap **[H scale]** on the touch screen to turn on/off the function.

6.3.2.24 Center Line

Display or hide a centerline which is used for needle guidance.

Operation:

Tap **[Center Line]** on the touch screen to display or hide the centerline.

NOTE: Centerline is only available for convex probes.

6.4 M-mode

M-Mode is used to determine patterns of motion for objects along the M-line. The most common use is for viewing motion patterns of the heart.

6.4.1 Basic Procedure of M-mode

To perform an M-mode imaging:

1. Optimize the B-mode image to make the image sharper.
2. Press the **[M]** knob on the control panel to enter the pre-active M-mode, and M-line is displayed on the B-mode image.
3. Roll the trackball to adjust the position of the M-line.
4. Press the **[M]** knob or the **[Update]** button on the control panel to enter the M-mode. The image is divided into two parts: B-mode image at the top and M-mode image at the bottom.
 - X axis: displays time
 - Y axis: displays the tissue position or depth
5. Move the M-line on B-mode image with the trackball; you can learn the movement of the anatomy along the M-line in the M-mode image.
6. Optimize the M-mode image. Refer to “6.4.2 Image Optimization (M)” for details.

The parameter area on the right side of the screen provides real-time parameter information of the M-mode. The meanings of each parameter are as follows:

Parameter	M-mode
F	Working Frequency (MHz)
D	Depth
G	Gain (dB)
V	Velocity
DR	Dynamic Range

7. Perform measurements and calculations as needed.

6.4.2 Image Optimization (M)

The screen displays the relevant imaging parameters and image options.

You can optimize the M image by tapping the corresponding parameter on the touch screen or by rotating/pressing the corresponding knob on the control panel.

6.4.2.1 Gain

The gain is used to adjust the brightness of the M image. You can brighten the image and observe more echo signals by increasing the gain. However, with increased gain, more noise would be introduced.

Operation:

In M-mode, rotate the **[M]** knob on the control panel to adjust the gain value.

6.4.2.2 Dynamic Range

Change the display range of the grayscale to adjust the contrast of the image.

Operation:

Rotate the knob under **[Dyn Ra.]** to adjust the dynamic range.

6.4.2.3 Gray Map

Optimize the images by adjusting the black-white contrast of the image.

Operation:

Rotate the knob under **[Gray Map]** to adjust the gray map.

6.4.2.4 Speed

Control the scanning speed of M mode imaging.

Operation:

Rotate the knob under **[Speed]** to adjust the M speed.

6.4.2.5 Chroma

Replace grayscale distinction with color distinction to intuitively show grayscale level of the images.

Operation:

Rotate the knob under **[Chroma]** to change the selection color.

6.4.2.6 Display Format

Change the display format of B image and M image for easy comparison of images.

Operation:

Tap **[Display Format]** on the touch screen to select the appropriate display format.

6.5 Color Mode

Color mode is also a Doppler mode to provide blood flow information in colors. Color mode includes basic color mode and PDI mode.

NOTE: Acoustic power in Color mode is synchronous with that of B-mode. Tap the mode tab on the touch screen to toggle the imaging modes.

6.5.1 Basic Procedure of Color Mode

The Color mode is used to visually detect the direction and speed of blood flow in the vessels. Typically, the color above the color bar baseline indicates the flow towards the probe; while color below the color bar baseline indicates the flow away from the probe.

The brighter the color, the faster the blood flows; the darker the color, the slower the blood flows.

To perform a color mode imaging:

1. Observe the anatomical structure, adjust the B-mode image and probe to make the target area at the center of the B-mode image.
2. Press the **[C]** knob on the control panel to enter Color-mode.
3. Adjust the position and size of the ROI box.
 - Press the **[Set]** button to toggle the ROI box between solid line and dotted line status.
 - When the ROI box is solid line, roll the trackball to adjust the position of the ROI box.
 - When the ROI box is dotted line, roll the trackball to adjust the size of the ROI box.
4. Optimize the image. (Refer to “6.5.3 Image Optimization (Color/PDI)” for details)

The parameter area on the right side of the screen provides real-time parameter information of the Color mode. The meanings of each parameter are as follows:

Parameter	Color-mode
F	Working Frequency (MHz)
G	Gain (dB)
WF	Wall Filter
PRF	Pulse Repetition Frequency

5. Perform measurements and calculations as needed.
6. Press the **[C]** knob on the control panel to exit the Color mode.

6.5.2 Basic Procedure of PDI mode

Power Doppler Imaging (PDI) is used to show the presence or absence of blood flow and to reflect the density of red blood cells.

NOTE: PDI mode only provides perfusion information of blood flow, but cannot indicate the direction and speed of blood flow.

To perform a PDI mode imaging:

1. Observe the anatomical structure, adjust the B-mode image and probe to make the target area at the center of the B-mode image.
2. Press the **[PDI]** button on the control panel to enter PDI mode.
3. Adjust the position and size of the ROI box.
 - Press the **[Set]** button to toggle the ROI box between solid line and dotted line status.
 - When the ROI box is solid line, roll the trackball to adjust the position of the ROI box.
 - When the ROI box is dotted line, roll the trackball to adjust the size of the ROI box.
4. Optimize the image. (Refer to “6.5.3 Image Optimization (Color/PDI)”)

The parameter area on the right side of the screen provides real-time parameter information of the PDI mode. The meanings of each parameter are as follows:

Parameter	PDI-mode
F	Working Frequency (MHz)
G	Gain (dB)
WF	Wall Filter
PRF	Pulse Repetition Frequency

5. Perform measurements and calculations as needed.
6. Press the **[PDI]** button on the control panel to exit the PDI mode.

6.5.3 Image Optimization (Color/PDI)

The screen displays the relevant imaging parameters and image options.

You can optimize the color/PDI image by tapping the corresponding parameter on the touch screen or by rotating/pressing the corresponding knob on the control panel.

6.5.3.1 Gain

Adjust the overall sensitivity of flow signals.

Operation:

Rotate the **[C]** knob on the control panel to adjust the Color/PDI gain value.

6.5.3.2 Image Quality

Adjust the frequency of current selected probe in Doppler mode.

Operation:

- Rotate the knob under **[Image Quality]** to select the frequency.
- Fundamental frequency options: Pen (Penetration priority), Gen (General imaging), Res (Resolution priority).

6.5.3.3 Scale

Adjust the speed range of color flow by changing the PRF.

Operation:

Rotate the knob under **[Scale]** to adjust the PRF value.

NOTE: Select appropriate PRF to match the flow velocity. Aliasing may result if low PRF is used for high flow velocity or small signal lost may result if high PRF is used for low flow velocity.

6.5.3.4 Smooth

Suppress noise and smooth the image.

Operation:

Rotate the knob under **[Smooth]** to adjust the smooth level.

6.5.3.5 Persistence

Superimpose and average the images of adjacent frames to remove the noise and enhance the details.

Operation:

Rotate the knob under **[Persistence]** to adjust the persistence level.

6.5.3.6 Color Map

➤ **Color**

Multiple sets of color maps are provided to optimize color flow display. This system provides

multiple different maps for users to choose. The ordinary map is marked with “V” while 2D map is marked with “VV”. The chosen spectrum color map is displayed on the color bar on the right side of the screen.

Operation:

Rotate the knob under **[Color Map]** to choose the color map.

➤ **PDI**

Provide color image display effect parameters, including energy spectrum and directional energy spectrum. This system provides different effect maps for users to choose. The energy maps are P0-3 while the direction energy maps are dP0-3. Directional energy spectrum also shows the direction information of blood flow.

Operation:

Rotate the knob under **[Color Map]** to choose the color map.

6.5.3.7 Line Density

Line density determines the number of the ultrasonic scanning lines of a certain width or angle. An increase of line density will improve lateral resolution of the image, but this will also decrease the frame rate.

Operation:

Tap [**<**] / [**>**] of **[Line Density]** on the touch screen to adjust line density level.

6.5.3.8 Sensitivity

Reflect the ability to reflect minimal detectable blood flow which is used to adjust the accuracy of color flow display. The higher the sensitivity, the more sensitive the response to low-speed blood flow and small blood vessel signals, and the better the image quality.

Operation:

Tap [**<**] / [**>**] of **[Sensitivity]** on the touch screen to adjust the sensitivity.

6.5.3.9 Flow State

Optimize images of different blood flow states.

Operation:

Tap [**<**] / [**>**] of **[Flow State]** on the touch screen to adjust the flow state.

6.5.3.10 Wall Filter

Filter low frequency noise to reduce the impacts of breathing and other activities.

Operation:

Tap [**<**] / [**>**] of **[Wall Filter]** on the touch screen to adjust the filtering value.

6.5.3.11 Baseline

Calibrate the 0 position of the color bar for the best blood flow speed display.

NOTE: Baseline function is unavailable for PDI mode.

Operation:

Tap [**<**] / [**>**] of [**Baseline**] on the touch screen to adjust the baseline.

6.5.3.12 Priority

Set the priority to displays blood flow information by color signals or gray signals.

The larger the value, color signals are prior to display; while the smaller the value, gray signals are prior to display.

Operation:

Tap [**>**] on touch screen to turn the page, and then tap [**<**] / [**>**] of [**Priority**] to adjust the color priority value.

6.5.3.13 Invert

Invert the color bar for blood flow direction.

By default, red color indicates the blood flow towards the probe; while blue color indicates the blood flow away from the probe. When the invert function is enabled, blue color indicates the blood flow towards the probe; while red color indicates the blood flow away from the probe.

The color flow image and the color bars on the right side of the image will change accordingly.

Operation:

- Tap [**Invert**] on the touch screen to turn on/off the invert function.
- Tap [**Auto-Invert**] on the touch screen to turn on/off the auto-invert function. (Only applicable for linear probes)

6.5.3.14 Dual Live

Display B and C images of one probe at the same time.

Operation:

Tap [**Dual Live**] on the touch screen to enable / disable the function of displaying B and C live images at the same time.

6.5.3.15 B/C Align

Set the maximum width of the B images the same width as the ROI box.

Operation:

Tap [**B/C Align**] on the touch screen to turn on/off the function.

6.5.3.16 Velocity Tag

Mark the flow at a specified velocity range for regional blood flow velocity observation.

- NOTE:**
- Only applicable for Color mode.
 - Press the **[Set]** button to switch between setting the marking position and selecting the marking range.

Operation:

1. Tap **[Velocity Tag]** on the touch screen to turn on/off the function.
 - A green mark appears on the color bar.
2. Roll the trackball to set the marking position.
3. Press the **[Set]** button to switch to marking range selection.
4. Roll the trackball to select the marking range.
 - The velocity within the marking range is displayed in the image parameter area.

6.5.3.17 Color Hide

Only black-and-white images are displayed when the color hiding function is on. Both color and black-and-white images are displayed when the function is off.

Operation:

Tap **[Color Hide]** on the touch screen to enable / disable the color hide function.

6.5.3.18 High Resolution Flow

Enhance the resolution of flow Image.

- NOTE:** Only applicable for Color mode.

Operation:

Tap **[HR Flow]** on the touch screen to turn on/off the function.

6.5.3.19 Flow Tracking

Locate flow automatically.

- NOTE:** Only applicable for linear probes.

Operation:

In Color mode, press the **[Auto]** knob on the control panel. The ROI box automatically locates the blood flow position, and the image is also optimized.

6.5.3.20 zMicroFlow

Display more vessel information, especially blood flow information of low-speed small vessels.

- NOTE:** Only applicable for PDI mode.

Operation:

Tap **[zMicroFlow]** on the touch screen to turn on/off the function.

6.5.3.21 Dynamic Range

Adjust the transformation of echo intensity into color signal.

NOTE: Not applicable for Color mode.

Operation:

In PDI mode, tap [**<**] / [**>**] of [**Dyn Ra.**] on the touch screen to adjust the dynamic range.

6.6 Doppler Imaging Mode

Doppler imaging is primarily used to provide blood flow velocity information and to indicate blood flow direction, type (e.g. arterial blood flow, venous blood flow) and properties.

Doppler imaging includes PW (Pulsed Wave Doppler) mode and CW (Continuous Wave Doppler) mode. PW mode displays regional blood flow velocity, direction and properties at a certain depth; CW mode is often used to display high-speed blood flow frequency. The combination of the two modes improves the accuracy of the diagnosis.

6.6.1 Basic Procedure of PW-mode

PW (Pulsed Wave Doppler) mode is used to learn the movement information of blood flow along a scanning line in a certain area. PW mode includes common pulse mode and high pulse repetition frequency (HPRF) mode.

To perform a PW-mode imaging:

1. Observe the anatomical structure, adjust the B-mode image and probe to make the target area at the center of the B-mode image.
2. Press the [**PW**] knob on the control panel to enter the pre-activated PW mode.

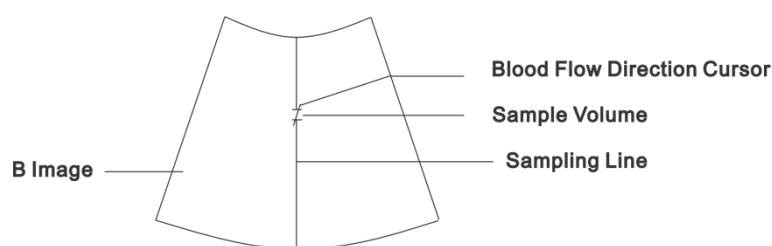


Figure 34 Pre-activated PW-mode

3. Adjust the sampling line and sampling depth to determine the sample volume in the target area.
 - Roll the trackball left and right to adjust the position of the sampling line.
 - Roll the trackball up and down to adjust the sample volume.
4. Adjust the sample volume and the cursor angle of blood flow direction.
 - Rotate the knob under [**SV**] to adjust the sample volume.
 - Rotate the [**Angle/Steer**] knob on the control panel to adjust the angle between the blood flow direction cursor and flow.

- You can also tap **[Quick Angle]** on touch screen to quickly switch among -60°, 0, 60°.
5. Press the **[PW]** knob or the **[Update]** button on the control panel to enter the PW-mode.

After entering PW-mode, the image area is divided into two parts: B-mode image at the top and PW-mode image at the bottom.

- The X axis indicates time.
 - The Y-axis indicates frequency change, and can also indicate the speed of forward or reverse direction after calibration.
 - Press the **[Update]** button on the control panel to toggle between B-mode and pre-activated PW-mode.
 - You can adjust the size and depth of sample volume and the cursor angle of the blood flow during exam.
 - Tap **[>]** on touch screen to turn the page, and then tap **[<] / [>]** of **[Volume]** to adjust the volume of the Doppler.
6. Optimize the image.(Refer to “6.6.3 Image Optimization (PW/CW)” for details)

The parameter area on the right side of the screen provides real-time parameter information of PW mode. The meanings of each parameter are as follows:

Parameter	PW-Mode
F	Working Frequency (MHz)
G	Gain (dB)
WF	Wall Filter
SVD	Sample Volume Depth
SV	Sample Volume
PRF	Pulse Repetition Frequency
Angle	Correction Angle

7. Perform measurements and calculations as needed to obtain valid information.
8. Press the **[PW]** knob on the control panel to exit the PW mode.

6.6.2 Basic Procedure of CW mode

The CW (Continuous Wave Doppler) mode collects blood flow signals and data along the spectral sampling line and is used to detect high-speed blood flow.

NOTE: CW mode is only available for phased array probes.

To perform a CW mode imaging:

1. Observe the anatomical structure, adjust the B-mode image and probe to make the target area at the center of the B-mode image.

2. Press the **[CW]** button on the control panel to enter the pre-activated CW-mode.

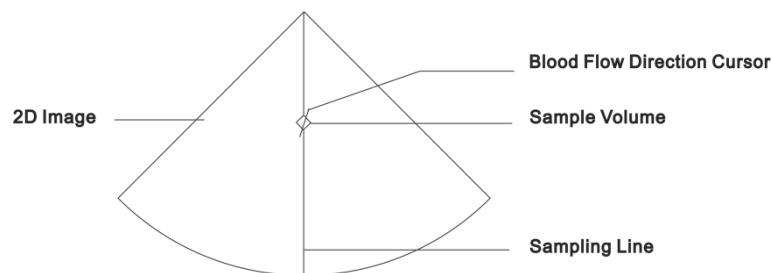


Figure 35 Pre-activated CW mode

3. Adjust the sampling line and sampling depth to determine the sample volume in the target area.
 - Roll the trackball left and right to adjust the position of the sampling line.
 - Roll the trackball up and down to adjust the sample volume.
4. Adjust the cursor angle of blood flow direction.
 - Rotate the **[Angle/Steer]** knob on the control panel to adjust the blood flow direction cursor angle.
 - You can also tap **[Quick Angle]** on touch screen to quickly switch among -60°, 0, 60°.
5. Press the **[CW]** button or the **[Update]** button on the control panel to enter the CW-mode.

After entering CW-mode, the image area is divided into two parts: B-mode image at the top and CW-mode image at the bottom.

- The X axis indicates time.
 - The Y-axis indicates frequency change, and can also indicate the speed of forward or reverse direction after calibration.
 - Press the **[Update]** button on the control panel to toggle between B-mode and CW-mode.
 - You can adjust the size and depth of sample volume and the cursor angle of the blood flow during exam.
 - Tap **[>]** on touch screen to turn the page, and then tap **[<] / [>]** of **[Volume]** to adjust the volume of the Doppler.
6. Optimize the image.(Refer to “6.6.3 Image Optimization (PW/CW)” for details)

The parameter area on the right side of the screen provides real-time parameter information of CW mode. The meanings of each parameter are as follows:

Parameter	CW Mode
F	Working Frequency (MHz)
G	Gain (dB)
WF	Wall Filter
SVD	Sample Volume Depth

Parameter	CW Mode
SV	Sample Volume
PRF	Pulse Repetition Frequency
Angle	Correction Angle

7. Perform measurements and calculations as needed.
8. Press the **[CW]** button on the control panel to exit the CW mode.

6.6.3 Image Optimization (PW/CW)

The screen displays the relevant imaging parameters and image options.

You can optimize the PW/CW image by tapping the corresponding parameter on the touch screen or by rotating/pressing the corresponding knob on the control panel.

6.6.3.1 Gain

Increase or decrease the echo signal strength displayed in the image.

Operation:

Rotate the **[PW]** knob on the control panel to adjust the PW/CW gain value.

6.6.3.2 Steer

Steer control is used to deflect the direction of beam without moving the probe.

NOTE: Applicable to linear probes only.

Operation:

Rotate the **[Angle/Steer]** knob on the control panel to adjust the direction of the ultrasonic beam.

6.6.3.3 Auto-optimization

The system automatically optimizes image parameters based on the tissue characteristics of the current scan area.

When auto-optimization function is enabled, an “Auto” mark is displayed in the image parameter area.

Operation:

Press the **[Auto]** knob on the control panel to enable/disable auto optimization.

6.6.3.4 Image Quality

Adjust the transmission frequency of the probe in Doppler mode. The higher the frequency, the higher the resolution and sensitivity, but the penetrating power is reduced. Select appropriate probe frequency based on the detection depth and tissue texture.

Operation:

- Rotate the knob under **[Image Quality]** to select the frequency.
- Options: Pen (Penetration priority), Gen (General imaging), Res (Resolution priority)

6.6.3.5 Scale

Adjust the speed range of color flow by changing the PRF.

Operation:

Rotate the knob under **[Scale]** to adjust the PRF value.

NOTE: Select appropriate PRF to match the flow velocity. Aliasing may result if low PRF is used for high flow velocity or small signal lost may result if high PRF is used for low flow velocity.

6.6.3.6 Sampling Volume (SV)

Adjust the width of sampling volume.

NOTE: Applicable to PW mode only.

Operation:

Rotate the knob under **[SV]** to adjust the sample volume.

6.6.3.7 Speed

Control the imaging speed. The smaller the value, the faster the speed is.

Operation:

Rotate the navigation knob to display **[Speed]**, and then rotate the knob under **[Speed]** to adjust the imaging speed.

6.6.3.8 Baseline

Calibrate the 0 position of the scale for the best blood flow speed display.

Operation:

Rotate the knob under **[Baseline]** to adjust the baseline.

6.6.3.9 Chroma

Replace grayscale distinction with color distinction to intuitively show grayscale level of the images.

Operation:

Tap **[<] / [>]** of **[Chroma]** on the touch screen to change the color.

6.6.3.10 Dynamic Range

Change the display range of the grayscale to adjust the contrast of the image.

Operation:

Tap [**<**] / [**>**] of [**Dyn Ra.**] on the touch screen to adjust the dynamic range.

6.6.3.11 Trace Area

Set the trace area of the Doppler wave in the spectrum map.

Operation:

Tap [**<**] / [**>**] of [**Trace Area**] on the touch screen to set the Doppler image tracing range.

6.6.3.12 Wall Filter

Filter low frequency noise to reduce the impacts of breathing and other activities.

Operation:

Tap [**<**] / [**>**] of [**Wall Filter**] on the touch screen to quickly adjust the filtering value.

6.6.3.13 Angle

Adjust the angle of the blood flow direction cursor.

Operation:

Rotate the [**Angle/Steer**] knob on the control panel to adjust the angle; or tap [**<**] / [**>**] of [**Quick Angle**] on the touch screen to adjust the angle faster by 60 degrees.

6.6.3.14 Auto Calculation

Trace the spectral Doppler wave and perform parameter calculations. The results of the automatic calculation will be displayed in the measurement results window.

In the real-time state, the automatic spectrum results obtained from the latest or more cardiac cycles are always displayed; in the frozen and cine replay state, the corresponding measurement results of the traced area are displayed.

Operation:

1. Tap [**>**] on touch screen to turn the page, and then tap [**Auto Calc**] on the touch screen to turn on the auto calculation function.
2. Tap [**Auto Calc Para**] on the touch screen to select the parameter items.
3. Tap [**<**] / [**>**] of [**Auto Calc Cycle**] on the touch screen to select the cardiac cycles for calculation.

6.6.3.15 T/F Resolution

Obtain quality images by adjusting time resolution and spatial resolution.

Operation:

Tap [**>**] on touch screen to turn the page, and then tap [**<**] / [**>**] of [**T/F Resolution**] to adjust the T/F resolution level.

6.6.3.16 Gray Map

Optimize the images by adjusting the black-white contrast of the image.

Operation:

Tap [**>**] on touch screen to turn the page, and then tap [**<**] / [**>**] of [**Gray Map**] to adjust the gray map.

6.6.3.17 Volume

Control and adjust the audio volume produced by the spectral Doppler which helps to determine the blood flow state and properties more effectively.

Operation:

Tap [**>**] on touch screen to turn the page, and then tap [**<**] / [**>**] of [**Volume**] to adjust the volume.

6.6.3.18 Invert

Flip the directions of the spectrum display.

Operation:

- Tap [**Invert**] on the touch screen to turn on/off the invert function.
- Tap [**Auto-Invert**] on the touch screen to turn on/off the auto-invert function. (Only applicable for linear probes)

6.6.3.19 Multi Sync

Display the PW image together with B image or with B+Color image at the same time.

NOTE: Applicable to PW mode only.

Operation:

Tap [**Multi Sync**] on the touch screen to turn on/off the function.

6.6.3.20 Display Format

Change the display format of B image and PW/CW image to facilitate comparison of images.

Operation:

Tap [**Display Format**] on the touch screen to select the appropriate display format.

6.6.3.21 High Pulse Repetition Frequency (HPRF)

HPRF mode is used when detected velocities exceed the processing capabilities of the currently selected PW Doppler scale, or when the selected anatomical site is too deep for the selected PW Doppler scale.

NOTE: Applicable to PW mode only.

Operation:

Tap [**HPRF**] on the touch screen to turn on/off HPRF function.

6.7 Anatomical M-mode

Anatomical M-mode imaging can analyze any part and direction of the 2D image, so as to obtain the myocardial motion trajectory of the region of interest. Tissue information can be evaluated more accurately and comprehensively by comparing multiple sampling lines and images at different times. The system supports both linear anatomical M-mode and curved anatomical M-mode.

NOTE: Anatomical M-images are provided for reference only. When diagnosing, please combine other clinical data for comprehensive analysis.

6.7.1 Linear Anatomical M-mode

To perform an Anatomical M-mode imaging:

1. Observe the anatomical structure, adjust the image and probe to make the target area at the center of the B-mode image.

Or perform the anatomical M-imaging on the desired 2D cine file.

2. In B or M-mode, tap **[Anatomical M]** on the touch screen or press the user-defined **"Anatomical M"** button to enter Anatomical M-mode. (For details of customizing a user-defined button, see "4.2.5 Customize".)

The A, B, and C sampling lines are displayed by default on the B mode image, and the M image shows the motion trajectories of the 3 sampling lines respectively.

3. Adjust sampling line. Green for activated while white for inactivated.
 - Position: roll the trackball to adjust the position of the sampling line.
 - Direction: rotate the **[Angle/Steer]** knob on the control panel to set the direction of the sampling line.
 - Display / Hide: tap **[Show A]**, **[Show B]** or **[Show C]** on the touch screen to display/hide the A, B, C sampling line. At least 1 sampling line shall be selected.
4. Optimize the image. (Refer to "6.4.2 Image Optimization (M)" for details)
5. Press the **[B]** knob on the control panel to exit the Anatomical M mode and return to the B-mode.

6.7.2 Curved Anatomical M-mode

NOTE: Only phased probe supports Curved Anatomical M-mode.

To perform a Curved Anatomical M-Mode imaging:

1. Before using anatomical M imaging, please set up user-defined button for anatomical M imaging. (Refer to "4.2.5 Customize")
2. In TVM mode (in M mode, press **<TDI>** and then press **[M]** or **[Update]** to enter the TVM mode), tap **[Anatomical M]** on the touch screen or press the user-

defined “**Anatomical M**” button to activate the Curved Anatomical M-mode. (For details of customizing a user-defined button, see “4.2.5 Customize”.)

3. Press the left **[Set]** button to define the start point of the sample line on the B image. The digital number "1" is marked beside the point.
4. Roll the trackball and press the left **[Set]** button to define the next point, and repeat to add more points.
5. Press the right **[Set]** button to finish the sample line.
6. Optimize the image as needed.

6.7.2.1 Edit the Curved Sample Line

To edit the curved sample line:

1. Tap **[Edit]** on the touch screen to enable curve (sample line) modification.
2. Move the cursor to a point to be modified, press the left **[Set]** button to activate the point, and then roll the trackball to drag the point as needed.
3. Repeat step 2 until a desired curve is achieved.
4. Press the right **[Set]** button to finish curve modification.

6.7.2.2 Delete the Curved sample line

Tap **[Delete]** on the touch screen to delete the current curve.

6.7.2.3 Undo the Point

Tap **[Undo]** on the touch screen to undo the last point.

6.8 Color M-mode

Color M-mode provides information of flow or tissue on the M-mode to indicate cardiac motion state.

For its sensitivities for motion signal changes, this mode provides more detailed diagnostic information.

To perform a Color M-mode imaging:

1. To enter the pre-activated Color M-mode:
 - **CFM (Color Flow M Mode)**
 - In B+M mode, press the **[C]** knob on the control panel.
 - In B+Color mode, B+Color+PW mode or B+Color+ CW mode, press the **[M]** knob on the control panel.
 - **TVM (Color Tissue M Mode)**
 - In CFM mode, press the **[Q2]** button on the control panel.
2. Adjust the color ROI box size and position.
 - Move the trackball left and right to adjust the position of sampling line, the color ROI box

moves together with the sampling line.

- Press the **[Set]** button to toggle between sampling line, solid line ROI box, and dotted line ROI box.
 - When the ROI box is solid line, roll the trackball to adjust the position of the ROI box.
 - When the ROI box is dotted line, roll the trackball to adjust the size of the ROI box.
3. Press the **[M]** knob or **[Update]** button on the control panel to enter the Color M mode.
 4. Optimize the Image. (For details, please refer to “6.4.2 Image Optimization (M)”.)

6.9 Tissue Doppler Imaging (TDI)

TDI mode is used to detect low-speed, high-intensity tissue motion information, so as to analyze myocardial wall motion.

NOTE: Applicable for phased array probes only.

6.9.1 TDI-modes

The ultrasonic system provides 4 tissue Doppler imaging modes for observing different tissue motion characteristics.

- TVI: to color code the speed and direction of the ventricular wall motion for myocardial velocity analysis.
- TEI: to color code the energy of the ventricular wall motion to observe myocardial blood supply.
- TVD: to display tissue motion within the ROI box in the direction of the sampled beam in the form of spectrogram for quantitative analysis of tissue motion.
- TVM: to provide intuitive color maps of tissue cardiogram and velocity information of myocardial motion.

6.9.2 Basic Procedure of TDI mode

To perform a TDI-mode imaging:

1. Enter the TDI mode.

In the real-time state of the following modes, press the user-defined TDI button (it is set to **[Q2]** by default; to customize a new TDI button, see “4.2.5 Customize”) to enter the corresponding TDI mode:

- In B or Color mode, press **[Q2]** to enter the TVI mode.
 - In PDI mode, press **[Q2]** to enter the TEI mode.
 - In PW pre-activated mode, press **[Q2]** and then press **[PW]** or **[Update]** to enter the TVD mode.
 - In M mode, press **[Q2]** and then press **[M]** or **[Update]** to enter the TVM mode.
2. Optimize the image.

3. Select TDI mode.
 - Press **[C]**, **[PW]**, **[M]**, **[PDI]** to toggle between the TDI modes.
4. Exit the TDI mode.

6.10 Panoramic Imaging

The panoramic imaging technology splices a series of real time 2D images into a continuous slice image, shows the whole picture of the anatomical region more intuitively and visually, and facilitates observation and measurement of the overall tissue texture. It is suitable for certain areas that require a larger field of view, such as the thyroid gland.

- NOTE:**
- **The Panoramic Imaging function is purchasable. Please confirm the function is purchased and installed before use.**
 - **Panoramic Images are provided for reference only. When diagnosing, please combine other clinical data for comprehensive analysis.**
 - **Panoramic imaging is an image splicing function. The quality of spliced images depends on the operator's technology to a certain extent. You may need to practice and master certain skills before you can get a satisfactory image. Therefore, there are certain risks in measurement.**

6.10.1 Basic Procedure of Panoramic Imaging

6.10.1.1 Precautions

- Make sure that the probe transducer and the scan path are evenly covered with enough coupling gel.
- Move the probe slowly and steadily.
- DO NOT shake, rotate or tilt the probe.
- DO NOT raise the probe or leave the skin surface, make sure that the probe is in vertical contact with the skin surface.
- DO NOT change the motion direction of the probe or move back and forth during scanning.
- Large scan depth usually requires a reduction in the probe moving speed.

6.10.1.2 Procedure

Perform the following steps:

1. In B or Color/PDI mode, tap **[Pano]** on the touch screen or press the user-defined "Pano" button to enter the pre-activated panoramic imaging move. (For details of customizing a user-defined button, see "4.2.5 Customize".) The ROI box displays on the image.
2. Adjust the position and size of the ROI box.
 - Press the **[Set]** button to toggle the ROI box between solid line and dotted line status.
 - When the ROI box is solid line, roll the trackball to adjust the position of the ROI box.
 - When the ROI box is dotted line, roll the trackball to adjust the size of the ROI box.

3. Tap **[Start Acquisition]** on the touch screen or press the **[Update]** button on the control panel to activate the acquisition state.
 - The image area displays two images; the upper image shows the real-time 2D image while the lower image shows the real-time spliced image.
4. Slowly and smoothly move the probe along the scanning section to acquire image. When collecting images, please pay attention to the color of the ROI box and adjust the moving speed properly.
 - Green: appropriate speed.
 - Blue: too slow.
 - Red: too fast.
5. Tap **[End Acquisition]** on the touch screen to end the acquisition, and the spliced image displayed in the image area.
6. Optimize the image. (Refer to “6.10.2 Image Optimization (Pano)” for details)
7. View and manage images.
 - Zooming: Rotate the **[Zoom]** knob on the control panel to zoom in/out the image globally.
 - Rotation: Rotate the **[Angle/Steer]** knob on the control panel to rotate the panorama image.
 - Perform measuring or add body marks or annotations as desired.
8. Press the **[B]** knob on the control panel to exit the panoramic imaging mode and return to B-mode.

6.10.2 Image Optimization (Pano)

6.10.2.1 Chroma

Replace grayscale distinction with color distinction to intuitively show grayscale level of the images.

Operation:

Rotate the knob under **[Chroma]** to change the color.

6.10.3 Image Quality

Panoramic images shall be combined with other clinical methods in diagnosis. Before using or measuring an image, make sure that the acquired image is clear and reliable.

Reacquire the image in the case of any one of the following situation happens:

- The image capture source is not a single plane.
- There is large black area in the image.
- Non continuous image.
- There are shadows in the image.
- Non continuous skin line.
- Unclear anatomical contour.

6.11 Elastography

Elastography indicates the elastic property distribution of the tissue by manual pressure or human breathing, and quantitatively displays the relative hardness of the tissue, thereby judging the hardness of the mass.

- NOTE:**
- **The Elastography function is purchasable. Please confirm the function is purchased and installed before use.**
 - **Elastography is only available for linear array probes.**

6.11.1 Basic Procedure of Elastography

Perform the following steps:

1. In B-mode, tap **[Elasto]** on the touch screen or press the user-defined “Elasto” button to enter the Elastography mode. (For details of customizing a user-defined button, see “4.2.5 Customize”.)
 - The image area displays two real-time images on the left and right; the left is elastography image with ROI box while the right is the real-time B image. The pressure curve is displayed in real time at the bottom of the screen.
 - X-axis indicates time and Y-axis indicates pressure level.
2. Adjust the position and size of the ROI box.
 - Press the **[Set]** button to toggle the ROI box between solid line and dotted line status.
 - When the ROI box is solid line, roll the trackball to adjust the position of the ROI box.
 - When the ROI box is dotted line, roll the trackball to adjust the size of the ROI box.
3. Optimize the image.(Refer to “6.11.2 Image Optimization (Elastography)” for details)

The parameter area on the right side of the screen provides real-time parameter information of Elastography mode. The meanings of each parameter are as follows:

Parameter	Description
MAP	Map
OP	Opacity

4. View and manage images.
5. Press the **[B]** knob on the control panel to exit the Elastography imaging mode and return to B mode.

6.11.2 Image Optimization (Elastography)

6.11.2.1 Persistence

Superimpose and average the images of adjacent frames to remove the noise and enhance the details.

Operation:

Rotate the knob under **[Persistence]** to adjust the persistence level.

6.11.2.2 Smooth

Suppress noise and smooth the image.

Operation:

Rotate the knob under **[Smooth]** to adjust the smooth level.

6.11.2.3 Opacity

Adjust the opacity of the image.

Operation:

Rotate the knob under **[Opacity]** to change the opacity of the image.

6.11.2.4 Map

Display different color maps and toggle the map between color and gray for better observation.

Operation:

Rotate the knob under **[Map]** to choose the map.

6.11.2.5 Invert

Flip the map.

Operation:

Tap **[Invert]** on the touch screen to turn on/off the invert function.

6.11.2.6 Synchronization

Switch the display between dual image (B+Elasto) and B-mode image.

Operation:

- Tap **[Sync]** on the touch screen to enables/disables synchronized display of live B-mode images and Elasto image function.
- When enabled, two image windows are displayed in the image area, with the 2D+Elasto image on the left side and the 2D image on the right side; when disabled, only the 2D+Elasto image window is displayed.

Chapter 7 Image Review and Management

After the image acquisition is complete, you can view and compare the image by splitting display, image zooming, cine replay, etc., or you can perform other operations on the image, such as adding comments and body marks to the image.

7.1 Splitting Display

Dual-split display or Quad-split is used for ultrasound images comparison at different timing.

7.1.1.1 Dual-Split Display

1. In B-mode, press **[Dual]** button on the control panel to enter the dual-split mode. The image on the left displays the real-time B-image.
2. Press **[Dual]** button again, the image on the left will be frozen while the image on the right displays the real-time B image.

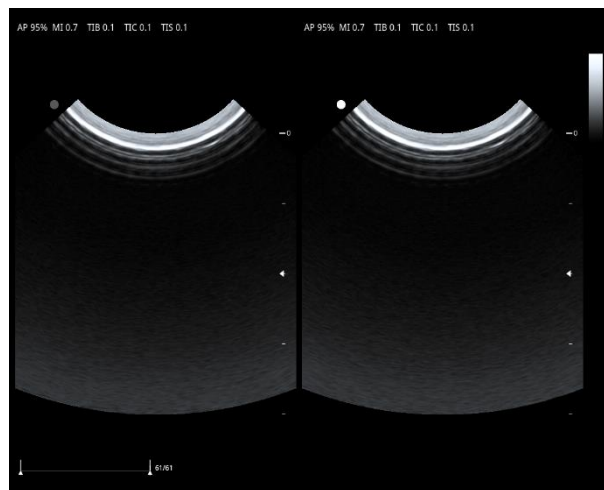


Figure 36 Dual-Split Display

3. Press the **[Dual]** button on the control panel to switch the real-time/frozen status of the left and right images.
4. Press the **[B]** knob on the control panel to exit dual-split display.

7.1.1.2 Quad-Split Display

1. Tap **[Quad]** on the touch screen to enter the Quad-Split display status which divides the image area into four equal areas.

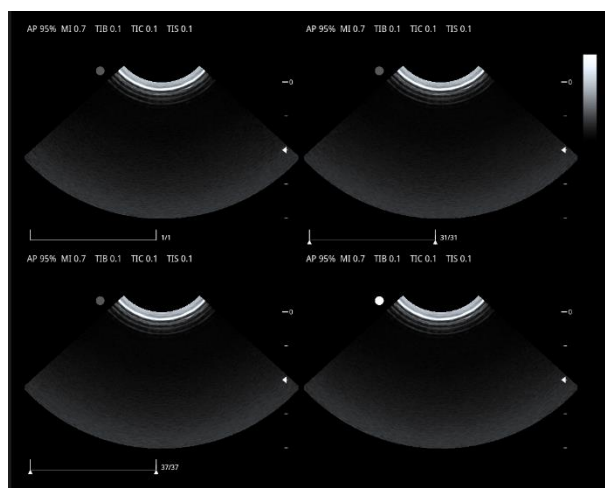


Figure 37 Quad-Split Display

2. Tap **[Quad]** again to freeze the current image and make the next image into real-time status.
3. Press the **[B]** knob on the control panel to exit Quad-Split display.

7.2 Image Magnification

Magnify the image to show more details.

- NOTE:**
- Image zooming changes the frame rate which tends to change the thermal index and position of the focus area and possibly results in different positions of the peak intensity in the acoustic field. As a result, the MI may change.
 - Adjust the position of the scale or focus as needed.

7.2.1 Global Zoom

1. Rotate the **[Zoom]** knob on the control panel to zoom the ultrasonic image.
2. Press the **[Zoom]** knob to exit global zooming.

7.2.2 Local Zoom

NOTE: Local zooming is only applicable to real-time images.

1. Press the **[Zoom]** knob on the control panel to activate local zoom function and display the ROI box.
2. Roll the trackball to adjust the position and size of ROI, press the **[Set]** button.
 - Press the **[Set]** button to toggle the ROI box between solid line and dotted line status.
 - When the ROI box is solid line, roll the trackball to adjust the position of the ROI box.
 - When the ROI box is dotted line, roll the trackball to adjust the size of the ROI box.
3. Rotate the **[Zoom]** knob on the control panel to zoom the ROI image.

4. Press the **[Zoom]** knob again to exit local zooming.

7.2.3 Fullscreen

1. Press **<FZoom>** on the keyboard to fullscreen display the ultrasonic image and parameter area.
2. Press **<FZoom>** again to fullscreen display the ultrasonic image.
3. Press **<FZoom>** again to exit fullscreen display function.

NOTE: Use the **<FZoom>** key to toggle the three display states in sequence.

7.3 Freeze the Image

You can freeze the image for next operation during the scanning at any time.

1. Press the **[Freeze]** on the control panel to freeze the image. Image zooming, measurement, annotation and optimization of some imaging parameters can be performed in the frozen state.
2. After freezing an image, the system may enter cine replay, caliper measurement or application measurement which depends on user's preset. For details, refer to "4.2.3 Image".
3. Press the **[Freeze]** again on the control panel to unfreeze the image.

NOTE: In Dual-Split display or Quad-Split display mode, only image of the currently activated window can be unfrozen, the other images remain frozen.

7.4 Cine Replay

In the real-time state, press the **[Freeze]** button on the control panel to freeze the current image and enter the cine replay by default, and the cine progress bar is displayed on the screen. You can review the cine repeatedly by automatic replay, or you can review the cine manually by rolling the trackball frame by frame.

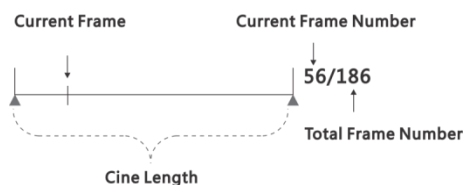


Figure 38 Cine Progress Bar (2D)

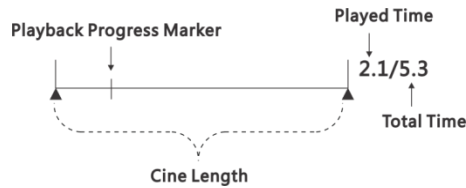


Figure 39 Cine Progress Bar (M/PW/CW/TVD)

Table 27 Cine Replay Operation

Item	Description
Save	Click to save cine region.
Reset	Click to reset the first frame and last frame.
Jump to First	Jump to the first frame.
Jump to Last	Jump to the last frame.
Start Frame	Set the start frame.
End Frame	Set the end frame.
Start Time	Set the start time.
End Time	Set the end time.
Replay speed	Set the replay speed.

NOTE: System defaults to replay cine manually.

7.4.1 Cine Replay Region

To set the cine replay region, please perform the following steps:

➤ **2D Mode:**

1. Rotate the knob under the **[Start Frame]** or roll the trackball to desired frame and then press left set button to set the start point of the cine replay region.
2. Rotate the knob under the **[End Frame]** or roll the trackball to desired frame and then press right set button to set the end point of the cine replay region.

➤ **M/PW/CW/TVD Mode:**

1. Rotate the knob under the **[Start Time]** or roll the trackball to desired frame and then press left set button to set the start time of the cine replay region.
2. Rotate the knob under the **[End Time]** or roll the trackball to desired frame and then press right set button to set the end time of the cine replay region.

NOTE:

- The system plays the cine replay region automatically after replay region setting.
- Press the **[Save 2]** button on the control panel to save the cine replay region to the clipboard.

7.4.2 Manual Replay

After entering the cine replay, roll the trackball to replay the cine frame by frame. The progress bar shows the position of the current frame.

Manual replay can be performed in the replay region.

7.4.3 Auto Replay

➤ Enable Auto Replay

- In the manual replay status, press the knob under the **[Replay Speed]** to enable auto replay, or rotate the knob under the **[Replay Speed]** to adjust the replay speed to enable the auto replay.

➤ Disable Auto Replay

- In the auto replay status, press the knob under the **[Replay Speed]** to disable auto replay, or rotate the knob under the **[Replay Speed]** to **[Off]** to disable auto replay and switch to the manual replay.
- In the auto replay status, roll the trackball to disable auto replay and switch to the manual replay.

NOTE: The system plays the cine replay region automatically after replay region has been set.

7.5 Annotation

Annotation function provides comment, arrow and body mark functions to the image. Comment, arrow and body mark are available to the ultrasound images in frozen and real-time states.

NOTE: Users can preset annotation via **[System Preset] → [Application]**. Refer to “4.2.4 Application” for details.

7.5.1 Comment

Users can enter text content directly or add comment item to images.

7.5.1.1 Add Comment

To add a comment, please perform the following steps:

1. Press the **[ABC]** button on the control panel or the **<Text>** key on the keyboard in any modes to activate comment function.
2. Select comment language, comment library and comment size.
 - Rotate the knob under **[English]** to switch text language between Chinese and English.
 - Rotate the knob under **[Exam]** to preset comment item library.
 - Rotate the knob under **[Font Size]** to set text size.

3. Click comment item you want to add, roll the trackball to move the comment item to the desired position, press the **[Set]** button.
4. If there is no applicable comment item, roll the trackball to move the comment item to the desired position and enter the comment through keyboard, and press the **[Set]** button. Or you can add a new comment item by customizing comment. (Refer to "7.5.1.2 Customize Comment" for details)
5. To add more comments, repeat Step 3 and 4.
6. Press **[ABC]** button on the control panel or press **<Fn> + <Text>** key on the keyboard to exit comment function.

7.5.1.2 Customize Comment

1. Tap **[Custom]** on the touch screen to enter the custom comment interface.
2. Add comments, delete comments, or adjust the position of comments as needed.
 - Add a comment: Enter the comment in the custom text box and click **[Add]**.
 - Delete a comment: Select a comment to be deleted and click **[Delete]**.
 - Adjust the position of comments: Click on two comments in sequence to swap their positions.
3. Click **[OK]** to save the settings and exit the custom comment interface.

7.5.1.3 Edit Comment

1. Move the cursor over the comment item to activate the item. Activated comment item or text is highlight in green.
2. Move the cursor to the character to be modified by arrow keys of the keyboard.
3. Press **<Back>** to delete undesirable characters and enter new comments directly. After the modification, move the cursor away from the text comment to complete the modification.

7.5.1.4 Move Comment

1. Move the cursor to the text comment to be moved, press the **[Set]** button, the text comment is highlighted with green box.
2. Roll the trackball to move the text comment to the desire position, press the **[Set]** button.

7.5.1.5 Change Font Size

Rotate the knob under the **[Font Size]** to change the font size. Or you can change the font size through Preset screen (press**<Setup>**). Refer to "4.2.4 Application" for details.

7.5.1.6 Hide/Display Comment

Tap **[Hide]** / **[Display]** on the touch screen to hide or display comments.

7.5.1.7 Delete Comment

➤ Delete Selected Comment

1. In annotation screen, move the cursor over the comment to be deleted, press the **[Set]** button.
2. Press the **[Clear]** button on the control panel to delete the selected comment.

➤ Delete Recently-added Comment

In annotation screen, press the **[Clear]** button on the control panel to delete recently-added comment in reverse order.

➤ Delete All Comments

Long press the **[Clear]** button on the keyboard to delete all comments.

7.5.2 Arrow

7.5.2.1 Add Arrow

To add an arrow, please perform the following steps:

1. Press the **<Arrow>** key on the keyboard in any modes to activate arrow function.
2. Rotate the knob under **[Arrow Size]** to change the arrow size.
3. Rotate the **[Angle/Steer]** knob on the control panel to adjust the direction of the arrow.
4. To add more arrows, repeat step 2~4.
5. Move the cursor to the desire position, press the **[Set]** button.
6. Press the **<Arrow>** key on the keyboard again to exit arrow function.

7.5.2.2 Hide/Display Arrow

Tap **[Hide]** / **[Display]** on the touch screen to hide or display arrows.

7.5.2.3 Delete Arrow

- In annotation screen, press the **[Clear]** button on the control panel to delete the recently-added arrow in reverse order.
- Long press the **[Clear]** button on the control panel to delete all arrow marks.

7.5.3 Body Mark

7.5.3.1 Add Body Mark

To add a body mark, please perform the following steps:

1. Press the **<Body Mark>** key on the keyboard or the **[Body Mark]** button on the control panel in any modes to activate body mark function.
2. Rotate the knob under **[Exam]** to select body mark library.

3. Click the body mark you want to add.

NOTE: Click a new body mark on the touch screen / menu area to replace the current body mark.

4. Rotate the **[Angle/Steer]** knob on the control panel to adjust the direction of the body mark.
5. Press the **<Body mark>** on the keyboard again in any modes to exit body mark function.

7.5.3.2 Move Body Mark

1. Press the **[Cursor]** button on the control panel to display the cursor.
2. Move the cursor over the body mark to be moved, press the **[Set]** button. The cursor is displayed as a hand-shaped cursor.
3. Move the trackball to the desire position and press the **[Set]** button to place the body mark.

7.5.3.3 Delete Body Mark

In annotation screen, press the **[Clear]** button on the control panel to delete the body mark.

Chapter 8 Image Measurement

Measurement includes general measurement and application measurement. The system supports measurement in real-time, freeze, Dual-Split display, Quad-Split display, zooming and cine replay status.



Warning

- **Before making a measurement of the target area, make sure that the target area and image to be measured are correct and qualified to avoid misdiagnosis.**
- **Before performing Doppler color flow image measurement, do not let the probe emit direction perpendicular to the direction of blood flow, otherwise incorrect blood flow information may be displayed.**

NOTE: During the measurement, if the system has been powered off or the [EndExam] button on the control panel has been pressed, all unsaved data will be lost.

8.1 Basic Operating Procedure

To perform a measurement, please perform the following steps:

1. In the real-time or frozen status, press the **[Caliper]** or **[Measure]** button on the control panel to activate the general / application measurement function.
 - The menu area displays the general measurement menu/application measurement menu of the current exam mode, and the touch screen also displays the corresponding measurement menu.
2. Select measurement item.
 - Tap the measurement item on the touch screen or roll the trackball to select the measurement item and press the **[Set]** button.
3. Perform a measurement:
 - Move the cursor to the target area, press the **[Set]** button to activate measurement item. At the same time, the result window displays with measurement results and calculation data.
4. Adjust the position of result window (if needed).
 - After measurement, place the cursor on the title bar of the result window to change the cursor into a hand cursor. Press the **[Set]** button, and roll the trackball to move the result window.
5. After the measurement is completed, press the **[Caliper]** or **[Measure]** button on the control panel to exit the general / application measurement function.

8.2 General Measurement

8.2.1 2D General Measurement

2D mode general measurement is applicable for general measurement of 2D mode such as B-mode, Color mode, PDI mode, panoramic mode, and elastography.

8.2.1.1 Distance (2D)

Measure the distance between two points.

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Distance]** in the measurement menu, and the cursor appears.
3. Move the cursor to the start point and press the **[Set]** button.
4. Move the cursor to the end point and press the **[Set]** button.
5. Results are displayed in the result window.

8.2.1.2 Area & Circumference

Measure the area and circumference of an enclosed area. Available measurement method includes Trace, Ellipse, Cross and Spline.

➤ Trace

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Trace]** in the measurement menu, and the cursor appears.
3. Move the cursor to the start point of the target area and press the **[Set]** button.
4. Roll the trackball to trace the outline of the target and press the **[Set]** button to fix the end point of the trace line.
5. Results are displayed in the result window.

➤ Ellipse

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Ellipse]** in the measurement menu, and the cursor appears.
3. Move the cursor to set the start point of the first axis of the ellipse and press the **[Set]** button.
4. Move the cursor to set the end point of the first axis of the ellipse and press the **[Set]** button.
5. Roll the trackball to size the measured axis as needed and press the **[Set]** button.
6. Results are displayed in the result window.

➤ **Cross**

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Cross]** in the measurement menu, and the cursor appears.
3. Move the cursor to the start point of the target area and press the **[Set]** button.
4. Move the cursor to the end position of the fixed axis and press the **[Set]** button. An irregular circle appears on the screen.
5. Roll the trackball to set the start point of the second axis of the circle and press the **[Set]** button.
6. Roll the trackball to set the end point of the second axis of the circle and press the **[Set]** button.
7. Results are displayed in the result window.

➤ **Spline**

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Spline]** in the measurement menu, and the cursor appears.
3. Move the cursor to the start point of the target area and press the **[Set]** button.
4. Move the cursor along the target area to fix the second point and press the **[Set]** button.
5. Repeat step 4. A maximum of 12 points can be fixed.
6. Press the **[Set]** button twice to complete the measurement.
7. Results are displayed in the result window.

8.2.1.3 Angle

Measure the angle between two intersecting lines.

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Angle]** in the measurement menu, and the cursor appears.
3. Set two line segments as described in “8.2.1.1 Distance (2D)”.
4. The system automatically calculates the angle between the two line segments.
5. Results are displayed in the result window.

8.2.1.4 Volume

Measure the volume of the target object. Available measurement method includes 3 Dist, Ellipse and Ellipse Dist.

➤ **3 Dist**

To obtain the volume by measuring the vertical section area of the target object.

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Volume]** in the measurement menu, and the cursor appears.
3. Measures the length (D_1), width (D_2), and height (D_3) of the target object.
4. The system automatically calculates the volume. The length, width, height, and volume of the target object are displayed in the result window.
 - Formula: $\text{Volume (cm}^3\text{)} = \pi / 6 \times D_1 \text{ (cm)} \times D_2 \text{ (cm)} \times D_3 \text{ (cm)}$
 - D_1 , D_2 , and D_3 correspond to the length, width, and height of the target object.

➤ **Volume (Ellipse)**

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Volume (Ellipse)]** in the measurement menu, and the cursor appears.
3. Move the cursor to set the start point of the first axis of the ellipse and press the **[Set]** button.
4. Roll the trackball to set the end point of the first axis of the circle and press the **[Set]** button.
5. Move the cursor to adjust the second axis of the ellipse, and press the **[Set]** button to complete the volume ellipse measurement.
6. The system automatically calculates the volume. Results are displayed in the result window.
 - Formula: $\text{Volume (cm}^3\text{)} = \pi/6 \times a \text{ (cm)} \times b^2 \text{ (cm)}$
 - Where, “a” corresponds to the first axis of the ellipse, and “b” corresponds to the second axis of the ellipse.

➤ **Volume (E+Dist)**

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Volume (E+Dist)]** in the measurement menu, and the cursor appears.
3. Measure the area of the vertical section as described in “8.2.1.2 Area & Circumference”.
4. Move the cursor to set the start point of the third axis and press the **[Set]** button.
5. Move the cursor to set the end point of the third axis and press the **[Set]** button.
6. The system automatically calculates the volume. The area, length, and volume of the target object are displayed in the result window.
 - Formula: $\text{Volume (cm}^3\text{)} = \pi/6 \times a \text{ (cm)} \times b \text{ (cm)} \times m \text{ (cm)}$
 - Where, “a” corresponds to the long axis of the ellipse, and “b” corresponds to the short axis of the ellipse, “m” corresponds to the third axis of the ellipse.

8.2.1.5 Double Dist

Measure the distance between two mutually perpendicular lines.

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Double Dist]** in the measurement menu, and the cursor appears.
3. Move the cursor to set the start point of the first line segment and press the **[Set]** button.
4. Move the cursor to the end point of the line segment and press the **[Set]** button. A line perpendicular to the line segment is displayed on the screen.
5. Move the trackball to adjust the start point of the vertical line segment and press the **[Set]** button.
6. Move the trackball to adjust the end point of the vertical line segment and press the **[Set]** button.
7. Results are displayed in the result window.

8.2.1.6 Curve Length

Measure the length of a curve. Available measurement method includes Trace and Spline.

➤ Trace Len

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Trace Len]** in the measurement menu, and the cursor appears.
3. Move the cursor to the start point of the trace line and press the **[Set]** button.
4. Roll the trackball to trace the outline of the target and press the **[Set]** button to fix the end point of the trace line.
5. Results are displayed in the result window.

➤ Trace Len (Spline)

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Trace Len (Spline)]** in the measurement menu, and the cursor appears.
3. Move the cursor to the start point of the target area and press the **[Set]** button.
4. Move the cursor along the target area to fix the second point and press the **[Set]** button.
5. Repeat step 4. A maximum of 12 points can be fixed.
6. Press the **[Set]** button twice to set the end point of the spline.
7. Results are displayed in the result window.

8.2.1.7 Parallel

Measure the distance between five parallel lines on the ultrasound image.

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Parallel]** in the measurement menu, and the cursor and two lines perpendicular to each other appear.
3. Move the cursor to set the start point of the first parallel and press the **[Set]** button.
4. Move the cursor along the vertical line and press the **[Set]** button to set the second parallel.
5. Repeat step 4 to set the third, fourth, fifth parallel as needed.
6. Results are displayed in the result window.

8.2.1.8 B Hist

Measures and calculates the gray scale distribution of the ultrasonic echo signals in an enclosed region.

Available measurement method includes B Hist (Ellipse), B Hist (Trace), B Hist (Spline) and B Hist (Rectangle).

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[B-Hist (Ellipse)]**, **[B-Hist (Trace)]**, **[B-Hist (Spline)]** or **[B-Hist (Rectangle)]** in the measurement menu, and the cursor appears.
3. Set up an enclosed area with the area measurement method as described in "8.2.1.2 Area & Circumference".
4. The system automatically calculates the gray distribution of the ultrasonic echo signal in this area and displays it at the top of the screen.

8.2.1.9 B Profile

Measure and calculates the gray distribution of the ultrasonic echo signals across a line.

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[B Profile]** in the measurement menu, and the cursor appears.
3. Set a line with the distance measurement method as described in "8.2.1.1 Distance (2D)".
4. The system automatically calculates the gray distribution of the ultrasonic echo signal on the line and displays it at the top of the screen.

8.2.1.10 Depth

Measure the distance from the center of sector to the cursor (for surface probe) or the

distance from probe surface to the cursor in the direction of ultrasonic beam (for linear and convex array probe).

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Depth]** in the measurement menu, and the cursor appears.
3. Move the cursor to the desired position and press the **[Set]** button.
4. Results are displayed in the result window.

8.2.1.11 Color Vel

Measure the color flow velocity in Color mode.

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Color Vel]** in the measurement menu, and the cursor appears.
3. Move the cursor to the desired point for blood flow velocity measurement and press the **[Set]** button.
4. Rotate the **[Angle/Steer]** knob to align the floating line to make it consistent with the direction of blood flow.
5. Results are displayed in the result window.

8.2.1.12 Ratio (D)

Measure the lengths of any two lines and calculates their ratio.

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Ratio (D)]** in the measurement menu, and the cursor appears.
3. Set two line segments as described in “8.2.1.1 Distance (2D)”.
4. The system automatically calculates the ratio, and the results are displayed in the result window.

8.2.1.13 Ratio (Area)

Measure the areas of any two enclosed areas and calculates their ratio.

Perform the following steps:

1. Press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Ratio (Trace)]**, **[Ratio (Ellipse)]**, **[Ratio (Spline)]** or **[Ratio (Cross)]** in the measurement menu, and the cursor appears.
3. Use the area measurement method (choose one of trace, ellipse, spline, cross) to set two closed areas.
4. The system automatically calculates the ratio, and the results are displayed in the result window.

8.2.1.14 Strain Ratio

Measure the strain ratio in the image.

NOTE: Only Elastography imaging supports this function.

Perform the following steps:

1. In the Elastography imaging mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Strain Ratio]** in the measurement menu, and the cursor appears.
3. Perform the measurement as described in “8.2.1.13 Ratio (Area)”
4. After the measurement is complete, the measurement result will be displayed in the result window.

8.2.1.15 IMT

Measure the intima-media thickness of the carotid artery. Refer to “8.3.5.3 Vascular Study and Calculation” for details.

8.2.1.16 Volume Flow

Measure the blood flow through a blood cross section per unit time. Refer to “8.2.3.7 Vol Flow” for details.

8.2.2 M General Measurement

M mode general measurement is applicable for general measurement of M images and anatomical M images.

8.2.2.1 HR (M)

Measures the time of N ($N \leq 8$) cardiac cycles and calculates the heart rate in M-mode imaging.

Perform the following steps:

1. Set the cardiac cycle.
 - Enter the Preset screen, select **[Preset]** → **[System Preset]** → **[Application]**
 - Select the number of cardiac cycles from the **[Cardiac Cycle]** drop-down list.
 - Click **[Save]** to save current setting and return to the Home screen.
2. In M-mode, press the **[Caliper]** button on the control panel to start measurement.
3. Click **[HR (M)]** in the measurement menu, and the cursor appears.
4. Move the cursor to the start point and press the **[Set]** button.
5. Move the cursor to set the end point in horizontal direction and press the **[Set]** button.
6. Results are displayed in the result window.

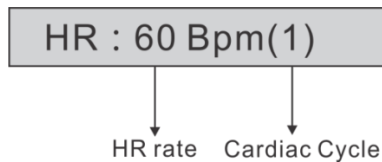


Figure 40 HR Result

NOTE: During the HR measurement, the number of cardiac cycles between the start and end points must be consistent with the preset. Otherwise, misdiagnosis may occur.

8.2.2.2 Distance (M)

Measure the distance between two points on the sampling line at a certain time.

Perform the following steps:

1. In M-mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Distance (M)]** in the measurement menu, and the cursor appears.
3. Move the cursor to the start point and press the **[Set]** button.
4. Move the cursor to the end point and press the **[Set]** button.
5. Results are displayed in the result window.

8.2.2.3 Time (M)

Measure the time interval between two points.

Perform the following steps:

1. In M-mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Time (M)]** in the measurement menu, and the cursor appears.
3. Move the cursor to the start point and press the **[Set]** button.
4. Move the cursor to set the end point in horizontal direction and press the **[Set]** button.
5. Results are displayed in the result window.

8.2.2.4 Slope

Measures the depth and time between two points and calculates the slope.

Perform the following steps:

1. In M-mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Slope]** in the measurement menu, and the cursor appears.
3. Move the cursor to set the first point and press the **[Set]** button.
4. Move the cursor to set the second point and press the **[Set]** button.
5. Results are displayed in the result window.

8.2.2.5 Velocity

Calculate the average velocity by measuring the distance and time between two points.

1. In M-mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Velocity]** in the measurement menu, and the cursor appears.
3. Move the cursor to the desired position and press the **[Set]** button.
4. Results are displayed in the result window.

8.2.3 Doppler General Measurement

Doppler general measurement is applicable for general measurement of PW/CW images.

8.2.3.1 Vel

Measures the velocity, pressure gradient and spectrum correction angle of a point on the Doppler spectrum waveform.

Perform the following steps:

1. In PW/CW mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Vel]** in the measurement menu, and the cursor appears.
3. Move the cursor, the real time velocity of the position is displayed in the result window. Move the cursor to the desired position and press the **[Set]** button.
4. Results are displayed in the result window.

8.2.3.2 Ratio (Vel)

Measures two D velocity and calculates their ratio for blood analysis.

Perform the following steps

1. In PW/CW mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Ratio (Vel)]** in the measurement menu, and the cursor appears.
3. Move the cursor to fix the two points for velocity measurement and press the **[Set]** button.
4. Move the cursor, the real time velocity of the position is displayed in the result window.
5. The velocity ratio of the two points is displayed in the result window.

- Formula: Vel Ratio (No unit) = | Vel 1(cm/s)/Vel 2 (cm/s) |

8.2.3.3 Time (Doppler)

Measure the time interval between two points.

Perform the following steps:

1. In PW/CW mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Time (Doppler)]** in the measurement menu, and the cursor appears.
3. Move the cursor to the start point and press the **[Set]** button.
4. Move the cursor to set the end point in horizontal direction and press the **[Set]** button.
5. Results are displayed in the result window.

8.2.3.4 HR (Doppler)

Measures the time of N ($N \leq 8$) cardiac cycles and calculates the heart rate in Doppler mode image. The measurement procedure is the same as that of HR (M). Refer to “0 M mode general measurement is applicable for general measurement of M images and anatomical M images.

HR (M)” for details.

8.2.3.5 D Trace

Trace one or several Doppler waveforms on the PW mode image to obtain speed and pressure gradient.

The Doppler spectrum diagram is shown below:

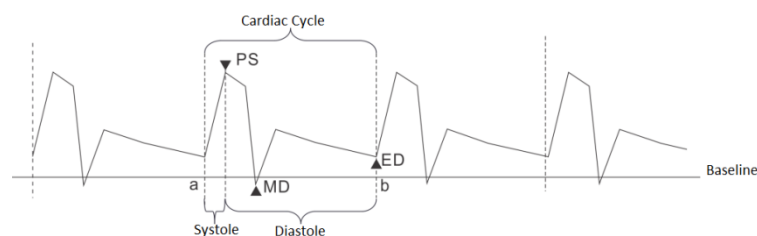


Figure 41 Doppler Spectrum

Perform the following steps:

1. In PW/CW mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[D Trace]** in the measurement menu, and the cursor appears.
3. Move the cursor to the start point and press the **[Set]** button.
4. Roll the trackball to draw a trace line along the spectrum Doppler waveform to the end position, and press the **[Set]** button to complete the trace. The measurement result is displayed in the result window.

The parameters displayed in the result window are described as follows:

Parameter	Description	
PS	Peak Systolic	The maximum velocity of red blood cells passing through the

Parameter	Description	
	Velocity	sampling volume
ED	End-diastolic velocity	The blood flow velocity at the end of the cardiac cycle
MD	Min-diastolic velocity	The minimum velocity of the cardiac cycle
Vel	/	Blood flow velocity
Average velocity	/	$TAMAX \text{ (cm/s)} = \int_{T_a}^{T_b} V(t)dt / (T_b - T_a)$ Where V is the maximum velocity $TAMEAN \text{ (cm/s)} = \int_{T_a}^{T_b} V(t)dt / (T_b - T_a)$ Where V is the average velocity
PPG	Peak Pressure Gradient	$PPG(\text{mmHg})=4 \times PS(\text{m/s})^2$
Average Pressure Gradient	Average Pressure Gradient	$MPG \text{ (mmHg)} = \int_{T_a}^{T_b} 4(V(t))^2 dt / (T_b - T_a)$ Where V is the peak systolic velocity $MMPG \text{ (mmHg)} = \int_{T_a}^{T_b} 4(V(t))^2 dt / (T_b - T_a)$ Where V is the average systolic velocity
VTI	Velocity-Time Integral	$VTI(m) = \int_{T_a}^{T_b} V(t)dt$
AT	Acceleration Time	Acceleration time from end-diastolic velocity to peak systolic velocity
DT	Deceleration Time	Deceleration time
HR	Heart rate	Beats per minute in a cardiac cycle
S/D	/	$S/D=PS(\text{m/s}) / ED(\text{m/s})$
D/S	/	$D/S = ED(\text{m/s}) / PS(\text{m/s})$
PI	Pulsatility Index	$PI = (PS(\text{m/s})-ED(\text{m/s})) / TAMAX(\text{m/s}) $
RI	Resistive	$RI = (PS(\text{m/s})-ED(\text{m/s})) / PS(\text{m/s}) $

Parameter	Description	
	Index	
θ	/	Correction Angle
PV	Peak Velocity	The maximum velocity of red blood cells passing through the sampling volume and it also applicable to venous vessels

8.2.3.6 PS/ED

Measures the velocity of peak systolic point (PS) and end diastolic (ED) on the Doppler spectrum.

1. In PW/CW mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[PS/ED]** in the measurement menu, and the cursor appears.
3. Move the cursor to the peak systolic velocity on the Doppler spectrum and press the **[Set]** button.
4. Move the cursor to the end diastolic velocity on the Doppler spectrum and press the **[Set]** button.
5. The RI, S/D and correction between the two points are displayed in the result window.

8.2.3.7 Vol Flow

Measure the blood flow through a blood cross section per unit time.

Perform the following steps:

1. In PW/CW mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Vol Flow]** in the measurement menu to display the sub-menu of volume flow: **[Vas Area]**, **[TAMEAN]**, and **[TAMX]**.
3. Click **[Vas Area]** in the measurement menu, rotate the knob under **[Vas Area]** to select measuring method as needed and the cursor appears.
4. Move the cursor to the start point of the target area on B-image and press the **[Set]** button.
5. Move the cursor to the end point of the target area on B-image and press the **[Set]** button.
6. The flow area is displayed in the result window.

NOTE: Steps 4 to 5 can also be performed in B-mode.

7. Click **[TAMEAN]** or **[TAMAX]** in the measurement menu, and the cursor appears.
8. Move the cursor to the start point of the target area on Doppler Spectrum and

press the **[Set]** button.

9. Move the cursor to the end point of the target area on Doppler Spectrum and press the **[Set]** button.
10. The system automatically generates trace lines. Results are displayed in the result window.

The parameters displayed in the result window are described as follows:

Parameter	Description	Formula
Vas Area	Dist	$\text{Vas Area} = \pi \times \text{Vas Diam (cm)}^2 / 4$
	Trace	See "8.2.1.2 Area & Circumference"
TAMEAN	Vol Flow(Area)-TAMEAN	$\text{Vol Flow(A) (ml/min)} = \text{Vas TAMEAN (cm/s)} \times \text{Vas Area (cm}^2) \times 60 \text{ (s)}$ Vas TAMEAN - Time Averaged Mean Velocity, obtained from Vas Trace measurement
TAMAX	Vol Flow(Area)-TAMAX	$\text{Vol Flow(A) (ml/min)} = \text{Vas TAMAX (cm/s)} \times \text{Vas Area (cm}^2) \times 60 \text{ (s)}$ Vas TAMAX - Time Averaged Maximum Velocity, obtained from Vas Trace measurement

8.2.3.8 Acceleration

Measure the velocity and time interval between two points on the Doppler image to calculate the acceleration, differential pressure, speed difference, and spectrum correction angle.

Perform the following steps:

1. In PW/CW mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Acceleration]** in the measurement menu, and the cursor appears.
3. Move the cursor to the first point and press the **[Set]** button.
4. Move the cursor to the second point and press the **[Set]** button.
5. The acceleration, differential pressure, speed difference, and spectrum correction angle between the two points are displayed in the result window.

8.2.3.9 Ratio (VTI)

Measure two VTI values and calculates their ratio.

Perform the following steps:

1. In PW/CW mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[Ratio (VTI)]** in the measurement menu, and the cursor appears.
3. Move the cursor to the start point of VTI1 and press the **[Set]** button.

4. Move the cursor to the end point of VT1 and press the **[Set]** button.
5. Repeat step 3~4 to fix the VT2.
6. The VT1, VT2, and VT ratio of the two points are displayed in the result window

- Formula: VT Ratio (No unit) = | VT 1(cm)/VT 2 (cm) |

8.3 Application Measurement

Application measurement package includes the following measurement items.

Table 28 Application Measurement Package

Application Measurement	Measurement Item
General	Applicable for general measurements.
Abdomen	Applicable for measurements of animal abdominal organs (liver, spleen, gallbladder, pancreas and kidney) and abdominal large blood vessels.
Reproduction	Applicable for measurement of animal fetus development indicators, GA and EDD estimation.
Cardiology	Applicable for measurement of cardiac and other parameters of animal.
Small Parts	Applicable for measurement of small organs such as thyroid, isthmus, testis and mass.
Vascular	Applicable for measurement of carotid, cerebral, upper and lower extremities vessels, etc.

8.3.1 Abdomen

8.3.1.1 2D Mode

The measurement items, calculation items and measurement method for 2D abdomen measurement are shown in the table below.

Table 29 2D Abdomen Measurement

Item		Description	Methods or Formula
Liver		/	See "8.2.1.1 Distance (2D)"
GB	GB L	Gallbladder Length	See "8.2.1.1 Distance (2D)"
	GB H	Gallbladder Height	See "8.2.1.1 Distance (2D)"
	GB wall th	Gallbladder Wall Thickness	See "8.2.1.1 Distance (2D)"

Item		Description	Methods or Formula
Adrenal	Adrenal L	Adrenal Length	See "8.2.1.1 Distance (2D)"
	Adrenal H	Adrenal Height	See "8.2.1.1 Distance (2D)"
	Adrenal W	Adrenal Width	See "8.2.1.1 Distance (2D)"
CHD		Common hepatic duct	See "8.2.1.1 Distance (2D)"
CBD		Common Bile Duct	See "8.2.1.1 Distance (2D)"
Portal V Diam		Portal Vein Diameter	See "8.2.1.1 Distance (2D)"
Pancreas	Panc head	Pancreatic Head	See "8.2.1.1 Distance (2D)"
	Panc body	Pancreatic Body	See "8.2.1.1 Distance (2D)"
	Panc tail	Pancreatic Tail	See "8.2.1.1 Distance (2D)"
	Panc duct	Pancreatic Duct	See "8.2.1.1 Distance (2D)"
	Pancreas	/	See "8.2.1.1 Distance (2D)"
Kidney	Renal L	Renal Length	See "8.2.1.1 Distance (2D)"
	Renal H	Renal Height	See "8.2.1.1 Distance (2D)"
	Renal W	Renal Width	See "8.2.1.1 Distance (2D)"
	Cortex	Renal Cortical Thickness	See "8.2.1.1 Distance (2D)"
	Renal Vol	Renal Volume	Measure Renal L, Renal H and Renal W, system then automatically calculates Renal Vol.
Spleen		/	See "8.2.1.1 Distance (2D)"
Aorta Diam		Aorta Diameter	See "8.2.1.1 Distance (2D)"
Iliac Diam		Iliac Diameter	See "8.2.1.1 Distance (2D)"
Prostate	Prostate L	Prostate Length	See "8.2.1.1 Distance (2D)"
	Prostate H	Prostate Height	See "8.2.1.1 Distance (2D)"
	Prostate W	Prostate Width	See "8.2.1.1 Distance (2D)"
Seminal Vesicle	Seminal L	Seminal Length	See "8.2.1.1 Distance (2D)"
	Seminal H	Seminal Height	See "8.2.1.1 Distance (2D)"
	Seminal W	Seminal Width	See "8.2.1.1 Distance (2D)"
Bladder	Pre-BL L	Pre-void Bladder Length	See "8.2.1.1 Distance (2D)"
	Pre-BL H	Pre-void Bladder Height	See "8.2.1.1 Distance (2D)"

Item		Description	Methods or Formula
	Pre-BL W	Pre-void Bladder Width	See "8.2.1.1 Distance (2D)"
	Pre-BL Vol	Pre-void Bladder Volume	Measure Pre-BL L, Pre-BL H and Pre-BL W, system then automatically calculates the Pre-BL Vol.
	Post-BL L	Post-void Bladder Length	See "8.2.1.1 Distance (2D)"
	Post-BL H	Post-void Bladder Height	See "8.2.1.1 Distance (2D)"
	Post-BL W	Post-void Bladder Width	See "8.2.1.1 Distance (2D)"
	Post-BL Vol	Post-void Bladder Volume	Measure Post-BL L, Post-BL H and Post-BL W, system then automatically calculates Post-BL Vol.
	Mictur.Vol	Micturated Volume	Measure Pre-BL Vol and Post-BL Vol, system then automatically calculates Mictur.Vol.
Ureter		/	See "8.2.1.1 Distance (2D)"

8.3.1.2 Doppler Mode

Table 30 Doppler Abdomen Measurement

Items		Description	Methods or Formula
Renal Arterial	Ren A Org	Renal Artery Origin	See "8.2.3.5 D Trace"
	Arcuate A	Arcuate Artery	See "8.2.3.5 D Trace"
	Segment A	Segmental Artery	See "8.2.3.5 D Trace"
	Interlobar A	Interlobar Artery	See "8.2.3.5 D Trace"
	Renal A	Renal Artery	See "8.2.3.5 D Trace"
	M Renal A	Main Renal Artery	See "8.2.3.5 D Trace"
	Renal V	Renal Vein	See "8.2.3.5 D Trace"
ABD Arterial	Aorta	/	See "8.2.3.5 D Trace"
	Celiac Axis	/	See "8.2.3.5 D Trace"
	SMA	Superior Mesenteric Artery	See "8.2.3.5 D Trace"
	C Hepatic A	Common Hepatic Artery	See "8.2.3.5 D Trace"
	Hepatic A	Hepatic Artery	See "8.2.3.5 D Trace"
	Splenic A	Splenic Artery	See "8.2.3.5 D Trace"
ABD	IVC	Inferior Vena Cava	See "8.2.3.5 D Trace"

Items		Description	Methods or Formula
Venous	Portal V	Portal Vein	See “8.2.3.5 D Trace”
	M Portal V	Main Portal Vein	See “8.2.3.5 D Trace”
	Hepatic V	Hepatic Vein	See “8.2.3.5 D Trace”
	Lt Hepatic V	Left Hepatic Vein	See “8.2.3.5 D Trace”
	M Hepatic V	Middle Hepatic Vein	See “8.2.3.5 D Trace”
	Rt Hepatic V	Right Hepatic Vein	See “8.2.3.5 D Trace”
	Splenic V	Splenic Vein	See “8.2.3.5 D Trace”
	SMV	Superior Mesenteric Vein	See “8.2.3.5 D Trace”
RAR		Ratio of Renal Artery PS the Abdominal Aorta PS	$RAR(\text{no unit}) = \frac{\text{Renal A PS (cm/s)}}{\text{Aorta PS (cm/s)}}$
SMA/Ao		Ratio of Superior Mesenteric Artery PS and Abdominal Aorta PS	$SMA/Ao (\text{no unit}) = \frac{\text{SMA PS (cm/s)}}{\text{Aorta PS (cm/s)}}$
CA/Ao		Ratio of Celiac Axis PS and Abdominal Aorta PS	$CA/Ao (\text{no unit}) = \frac{\text{Celiac Axis PS (cm/s)}}{\text{Aorta PS (cm/s)}}$

8.3.2 Reproduction

NOTE: Before performing reproduction measurements, please make sure that the system date is accurate, otherwise, the GA and EDD will be calculated incorrectly.

8.3.2.1 2D Mode

The measurement items, calculation items and measurement method for 2D obstetrics measurement are shown in the table below.

Animal	Items	Description	Methods or Formula
Cat	Cat HD	Cat Head Diameter	See “8.2.1.1 Distance (2D)”
	Cat BD	Cat Body Cavity Diameter	See “8.2.1.1 Distance (2D)”
Dog	Dog CRL	Dog Crown Rump Length	See “8.2.1.1 Distance (2D)”
	Dog GS	Dog Gestational Sac Diameter	See “8.2.1.1 Distance (2D)”
	Dog HD	Dog Head Diameter	See “8.2.1.1 Distance (2D)”
	Dog BD	Dog Body Cavity Diameter	See “8.2.1.1 Distance (2D)”
Equine	Equine GS-H	Equine Gestational Sac Diameter Horizontal	See “8.2.1.1 Distance (2D)”
	Equine GS-V	Equine Gestational Sac	See “8.2.1.1 Distance (2D)”

Animal	Items	Description	Methods or Formula
		Diameter Vertical	
Bovine	Bovine CRL	Bovine Crown Rump Length	See "8.2.1.1 Distance (2D)"
	Bovine TD	Bovine Trunk Diameter	See "8.2.1.1 Distance (2D)"
	Bovine HD	Bovine Head Diameter	See "8.2.1.1 Distance (2D)"
Ovine	Ovine CRL	Ovine Crown Rump Length	See "8.2.1.1 Distance (2D)"
	Ovine BPD	Ovine Biparietal Diameter	See "8.2.1.1 Distance (2D)"
/	Body Length	/	See "8.2.1.1 Distance (2D)"

8.3.2.2 Doppler Mode

Items	Description	Methods or Formula
Umb A	Umbilical Artery	See "8.2.3.5 D Trace"
MCA	Middle Cerebral Artery	See "8.2.3.5 D Trace"
Fetal Ao	Fetal Aorta	See "8.2.3.5 D Trace"
Desc Aorta	Descending Aorta	See "8.2.3.5 D Trace"
Placenta A	Placental Artery	See "8.2.3.5 D Trace"
Duct Venos	Ductus Venosus	See "8.2.3.5 D Trace"

8.3.3 Cardiology

8.3.3.1 2D Mode

The measurement items, calculation items and measurement method for 2D cardiology measurement are shown in the table below.

Items	Description	Methods or Formula
Ao Diam(2D)	Aorta Diameter (2D)	See "8.2.1.1 Distance (2D)"
Ao Arch Diam(2D)	Aorta Arch Diameter (2D)	See "8.2.1.1 Distance (2D)"
Ao Asc Diam(2D)	Ascending Aorta Diameter (2D)	See "8.2.1.1 Distance (2D)"
Ao Desc Diam(2D)	Descending Aorta Diameter (2D)	See "8.2.1.1 Distance (2D)"
Ao Isthmus(2D)	Aorta Isthmus Diameter (2D)	See "8.2.1.1 Distance (2D)"
Ao st junct(2D)	Aorta ST junct Diameter (2D)	See "8.2.1.1 Distance (2D)"
Ao Sinus Diam(2D)	Aorta Sinus Diameter (2D)	See "8.2.1.1 Distance (2D)"

Items	Description	Methods or Formula
AVA	Aortic Valve Area	See “8.3.3.4 Cardiology Study and Calculation”
ASD Diam	Atrial Septal defect Diameter	See “8.2.1.1 Distance (2D)”
ACS(2D)	Aortic Valve Cusp Separation (2D)	See “8.2.1.1 Distance (2D)”
AV Diam	Aorta Valve Diameter	See “8.2.1.1 Distance (2D)”
Duct Art Diam	Ductus Arteriosus Diameter	See “8.2.1.1 Distance (2D)”
HR(Cube 2D)	Heart Rate(Cube 2D)	See “8.3.3.4 Cardiology Study and Calculation”
HR(Gibson 2D)	Heart Rate (Gibson 2D)	See “8.3.3.4 Cardiology Study and Calculation”
HR(Teich 2D)	Heart Rate (Teich 2D)	See “8.3.3.4 Cardiology Study and Calculation”
IVC Diam(Expir)	Inferior Vena Cava Inspiration Diameter	See “8.2.1.1 Distance (2D)”
IVC Diam(Insp)	Inferior Vena Cava expiration Diameter	See “8.2.1.1 Distance (2D)”
IVSd(2D)	Interventricular Septal thickness at end-diastole (2D)	See “8.2.1.1 Distance (2D)”
IVSs(2D)	Interventricular Septal thickness at end-systole (2D)	See “8.2.1.1 Distance (2D)”
LA Area	Left Atrium area	See “8.2.1.2 Area & Circumference”
LA Diam(2D)	Left Atrium Diameter (2D)	See “8.2.1.1 Distance (2D)”
LA Major	Left Atrium Major Diameter	See “8.2.1.1 Distance (2D)”
LA Minor	Left Atrium Minor Diameter	See “8.2.1.1 Distance (2D)”
LCA Diam	Left Coronary Artery Diameter	See “8.2.1.1 Distance (2D)”
LPA Diam(2D)	Left Pulmonary Artery Diameter (2D)	See “8.2.1.1 Distance (2D)”
LV Area(d)	Left Ventricular area at end-diastole	See “8.3.3.4 Cardiology Study and Calculation”
LV Area(s)	Left Ventricular area at end-diastole	See “8.3.3.4 Cardiology Study and Calculation”
Diastole(Cube 2D)	End-diastolic Left Ventricular Measurement (Cube 2D)	See “8.3.3.4 Cardiology Study and Calculation”
Diastole(Gibson 2D)	End-diastolic Left Ventricular Measurement (Gibson 2D)	See “8.3.3.4 Cardiology Study and Calculation”
Diastole(Teich 2D)	End-diastolic Left Ventricular Measurement (Teich 2D)	See “8.3.3.4 Cardiology Study and Calculation”
LV Major	Left Ventricular Major Diameter	See “8.2.1.1 Distance (2D)”

Items	Description	Methods or Formula
LV Minor	Left Ventricular Minor Diameter	See "8.2.1.1 Distance (2D)"
Systole(Cube 2D)	End-systolic Left Ventricular Measurement	See "8.3.3.4 Cardiology Study and Calculation"
Systole(Gibson 2D)	End-systolic Left Ventricular Measurement (Gibson 2D)	See "8.3.3.4 Cardiology Study and Calculation"
Systole(Teich 2D)	End-systolic Left Ventricular Measurement (Teich 2D)	See "8.3.3.4 Cardiology Study and Calculation"
LVIDd(2D)	Left Ventricular Internal Diameter at end-diastole (2D)	See "8.2.1.1 Distance (2D)"
LVIDd(Cube 2D)	Left Ventricular Internal Diameter at end-diastole (Cube 2D)	See "8.2.1.1 Distance (2D)"
LVIDd(Gibson 2D)	Left Ventricular Internal Diameter at end-diastole (Gibson 2D)	See "8.2.1.1 Distance (2D)"
LVIDd(Teich 2D)	Left Ventricular Internal Diameter at end-diastole (Teich 2D)	See "8.2.1.1 Distance (2D)"
LVIDs(2D)	Left Ventricular Internal Diameter at end-systole (2D)	See "8.2.1.1 Distance (2D)"
LVIDs(Cube 2D)	Left Ventricular Internal Diameter at end-systole (Cube 2D)	See "8.2.1.1 Distance (2D)"
LVIDs(Gibson 2D)	Left Ventricular Internal Diameter at end-systole (Gibson 2D)	See "8.2.1.1 Distance (2D)"
LVIDs(Teich 2D)	Left Ventricular Internal Diameter at end-systole (Teich 2D)	See "8.2.1.1 Distance (2D)"
LVOT Diam	Left Ventricular Outflow Tract Diameter	See "8.2.1.1 Distance (2D)"
RVOT Diam	Right Ventricular Outflow Tract Diameter	See "8.2.1.1 Distance (2D)"
LVPWd(2D)	Left Ventricular Posterior wall thickness at end-diastole (2D)	See "8.2.1.1 Distance (2D)"
LVPWs(2D)	Left Ventricular Posterior wall thickness at end-systole (2D)	See "8.2.1.1 Distance (2D)"
MCS(2D)	Mitral Valve Cusp Separation (2D)	See "8.2.1.1 Distance (2D)"
MPA Diam(2D)	Main pulmonary Artery Diameter (2D)	See "8.2.1.1 Distance (2D)"
MVA	Mitral Valve Orifice Area	See "8.3.3.4 Cardiology Study and Calculation"
MV Diam	Mitral Valve Diameter	See "8.2.1.1 Distance (2D)"
MV EPSS(2D)	Distance between point E and Interventricular Septum when Mitral Valve is fully open (2D)	See "8.2.1.1 Distance (2D)"
PDA Diam	Patent Ductus Arteriosus Diameter	See "8.2.1.1 Distance (2D)"

Items	Description	Methods or Formula
PEd(2D)	Pericardial Effusion at diastole (2D)	See “8.2.1.1 Distance (2D)”
PEs(2D)	Pericardial Effusion at systole (2D)	See “8.2.1.1 Distance (2D)”
PFO Diam	Patent Oval Foramen Diameter	See “8.2.1.1 Distance (2D)”
Pre Ductal	Previous Ductal Diameter	See “8.2.1.1 Distance (2D)”
Post Ductal	Posterior Ductal Diameter	See “8.2.1.1 Distance (2D)”
PV Diam	Pulmonary Valve Diameter	See “8.2.1.1 Distance (2D)”
RA Area	Right Atrium Area	See “8.2.1.2 Area & Circumference”
RA Major	Right Atrium Major Diameter	See “8.2.1.1 Distance (2D)”
RA Minor	Right Atrium Minor Diameter	See “8.2.1.1 Distance (2D)”
RCA Diam	Right Coronary Artery Diameter	See “8.2.1.1 Distance (2D)”
RPA Diam(2D)	Right Pulmonary Artery Diameter (2D)	See “8.2.1.1 Distance (2D)”
RV Area(d)	Right Ventricular Area at end-diastole	See “8.2.1.2 Area & Circumference”
RV Area(s)	Right Ventricular Area at end-systole	See “8.2.1.2 Area & Circumference”
RV Major	Right Ventricular Major Diameter	See “8.2.1.1 Distance (2D)”
RV Minor	Right Ventricular Minor Diameter	See “8.2.1.1 Distance (2D)”
RVAWd(2D)	Right Ventricular Anterior Wall Thickness at end-diastole (2D)	See “8.2.1.1 Distance (2D)”
RVAWs(2D)	Right Ventricular Anterior Wall Thickness at end-systole (2D)	See “8.2.1.1 Distance (2D)”
RVDd(2D)	Right Ventricular Diameter at end-diastole (2D)	See “8.2.1.1 Distance (2D)”
RVDs(2D)	Right Ventricular Diameter at end-systole (2D)	See “8.2.1.1 Distance (2D)”
SVC Diam(Expir)	Superior Vena Cava Expiration Diameter	See “8.2.1.1 Distance (2D)”
SVC Diam(Insp)	Superior Vena Cava Inspiration Diameter	See “8.2.1.1 Distance (2D)”
TV Diam	Tricuspid Valve Diameter	See “8.2.1.1 Distance (2D)”
TVA	Tricuspid Valve Area	See “8.2.1.2 Area & Circumference”
VSD Diam	Ventricular Septal Defect Diameter	See “8.2.1.1 Distance (2D)”
HR(BP Ellipse)	Heart rate (BP Ellipse)	See “8.3.3.4 Cardiology Study”

Items	Description	Methods or Formula
		and Calculation”
LVAd sax MV(BP Ellipse)	Left ventricular area at mitral valve level at end-diastole in short-axis view (BP Ellipse)	See “8.2.1.2 Area & Circumference”
LVAs sax MV(BP Ellipse)	Left ventricular area at mitral valve level at end-systole in short-axis view (BP Ellipse)	See “8.2.1.2 Area & Circumference”
LVAd apical(BP Ellipse)	Left ventricular area at end-diastole in apical view (BP Ellipse)	See “8.2.1.2 Area & Circumference”
LVAs apical(BP Ellipse)	Left ventricular long axis length at end-systole in apical view (BP Ellipse)	See “8.2.1.2 Area & Circumference”
LVIDd(BP Ellipse)	Left Ventricular Internal Diameter at end-diastole (BP Ellipse)	See “8.2.1.1 Distance (2D)”
LVIDs(BP Ellipse)	Left Ventricular Internal Diameter at end-systole (BP Ellipse)	See “8.2.1.1 Distance (2D)”
HR(Bullet)	Heart rate (Bullet)	See “8.3.3.4 Cardiology Study and Calculation”
LVAd sax MV(Bullet)	Left ventricular area at mitral valve level at end-diastole in short-axis view (Bullet)	See “8.3.3.4 Cardiology Study and Calculation”
LVAs sax MV(Bullet)	Left ventricular area at mitral valve level at end-systole in short-axis view (Bullet)	See “8.3.3.4 Cardiology Study and Calculation”
LVLd apical(Bullet)	Left ventricular long axis length at end-diastole in apical view (Bullet)	See “8.3.3.4 Cardiology Study and Calculation”
LVLs apical(Bullet)	Left ventricular long axis length at end-systole in apical view (Bullet)	See “8.3.3.4 Cardiology Study and Calculation”
LA Diam(LA Vol A-L)	Left Atrium Diameter (Left Atrium Volume A-L)	See “8.2.1.1 Distance (2D)”
LAA(A2C)	Left Atrium Area at Apical 2-Chamber view	See “8.2.1.2 Area & Circumference”
LAA(A4C)	Left Atrium Area at Apical 4-Chamber view	See “8.2.1.2 Area & Circumference”
LA Vol(A2C)	Left Atrium Volume at Apical 2-Chamber view	See “8.3.3.4 Cardiology Study and Calculation”
LA Vol(A4C)	Left Atrium Volume at Apical 4-Chamber view	See “8.3.3.4 Cardiology Study and Calculation”
LVAd sax Epi(LV Mass A-L)	Left Ventricular Epicardial Area at Papillary Muscle level at end-diastole in Short-axis view (LV Mass A-L)	See “8.2.1.2 Area & Circumference”
LVAd sax Endo(LV Mass A-L)	Left Ventricular Endocardial Area at Papillary Muscle level at end-diastole in Short-axis view (LV Mass A-L)	See “8.2.1.2 Area & Circumference”

Items	Description	Methods or Formula
LVLd apical(LV Mass A-L)	Left Ventricular Long-axis Length at end-systole in apical view (LV Mass A-L)	See “8.2.1.1 Distance (2D)”
IVSd(LV Mass Cube-2D)	Interventricular Septal thickness at end-diastole (Left Ventricular Mass A-L Cube-2D)	See “8.2.1.1 Distance (2D)”
LVIDd(LV Mass Cube-2D)	Left Ventricular Internal Diameter at end-diastole (Left Ventricular Mass A-L Cube-2D)	See “8.2.1.1 Distance (2D)”
LVPWd(LV Mass Cube-2D)	Left Ventricular Posterior wall thickness at end-diastole (LV Mass A-L Cube-2D)	See “8.2.1.1 Distance (2D)”
LVA _d sax Epi(LV Mass T-E)	Left Ventricular Epicardial Area at Papillary Muscle level at end-diastole in Short-axis view (LV Mass T-E)	See “8.2.1.2 Area & Circumference”
LVA _d sax Endo(LV Mass T-E)	Left Ventricular Endocardial Area at Papillary Muscle level at end-diastole in Short-axis view (LV Mass T-E)	See “8.2.1.2 Area & Circumference”
a	/	See “8.2.1.1 Distance (2D)”
d	/	See “8.2.1.1 Distance (2D)”
RA Vol(A4C)	Right Atrium Volume at Apical 4-Chamber view	See “8.3.3.4 Cardiology Study and Calculation”
LVLd apical(SP Ellipse)	Left ventricular long axis length at end-diastole in apical view (SP Ellipse)	See “8.2.1.1 Distance (2D)”
LVA _d apical(SP Ellipse)	Left ventricular area at end-diastole in apical view (SP Ellipse)	See “8.2.1.2 Area & Circumference”
LVLs apical(SP Ellipse)	Left ventricular long axis length at end-systole in apical view (SP Ellipse)	See “8.2.1.1 Distance (2D)”
LVA _s apical(SP Ellipse)	Left ventricular area at end-systole in apical view (SP Ellipse)	See “8.2.1.2 Area & Circumference”
HR(SP Ellipse)	Heart rate (SP Ellipse)	See “8.3.3.4 Cardiology Study and Calculation”
LVLd apical(Simp)	Left ventricular long axis length at end-diastole in apical view (Simp)	See “8.2.1.1 Distance (2D)”
LVLs apical(Simp)	Left ventricular long axis length at end-systole in apical view (Simp)	See “8.2.1.1 Distance (2D)”
LVA _d sax MV(Simp)	Left ventricular area at mitral valve level at end-diastole in short-axis view (Simp)	See “8.2.1.2 Area & Circumference”
LVA _s sax MV(Simp)	Left ventricular area at mitral valve level at end-systole in short-axis view (Simp)	See “8.2.1.2 Area & Circumference”
LVA _d sax PM(Simp)	Left ventricular area at papillary muscle level at end-diastole in short axis view (Simp)	See “8.2.1.2 Area & Circumference”
LVA _s sax PM(Simp)	Left ventricular area at papillary muscle	See “8.2.1.2 Area &

Items	Description	Methods or Formula
	level at end-systole in short axis view (Simp)	Circumference"
HR(Mod Simp)	Heart rate (Mod. Simpson)	See "8.3.3.4 Cardiology Study and Calculation"
EDV(Simp BP-A2C)	End-diastolic Left Ventricular Volume (Simp BP-Apical 2-Chamber)	See "8.3.3.4 Cardiology Study and Calculation"
ESV(Simp BP-A2C)	End-systolic Left Ventricular Volume (Simp BP-Apical 2-Chamber)	See "8.3.3.4 Cardiology Study and Calculation"
EDV(Simp BP-A4C)	End-diastolic Left Ventricular Volume (Simp BP-Apical 4-Chamber)	See "8.3.3.4 Cardiology Study and Calculation"
ESV(Simp BP-A4C)	End-systolic Left Ventricular Volume (Simp BP-Apical 4-Chamber)	See "8.3.3.4 Cardiology Study and Calculation"
HR(Simp BP)	Heart Rate (Simp BP)	See "8.3.3.4 Cardiology Study and Calculation"
EDV(Simp SP-A2C)	End-diastolic Left Ventricular Volume (Simp SP-Apical 2-Chamber)	See "8.3.3.4 Cardiology Study and Calculation"
ESV(Simp SP-A2C)	End-systolic Left Ventricular Volume (Simp SP-Apical 2-Chamber)	See "8.3.3.4 Cardiology Study and Calculation"
HR(Simp SP A2C)	Heart Rate (Simp SP-Apical 2-Chamber)	See "8.3.3.4 Cardiology Study and Calculation"
EDV(Simp SP-A4C)	End-diastolic Left Ventricular Volume (Simp SP-Apical 4-Chamber)	See "8.3.3.4 Cardiology Study and Calculation"
ESV(Simp SP-A4C)	End-systolic Left Ventricular Volume (Simp SP-Apical 4-Chamber)	See "8.3.3.4 Cardiology Study and Calculation"
HR(Simp SP A4C)	Heart Rate (Simp SP-Apical 4-Chamber)	See "8.3.3.4 Cardiology Study and Calculation"
LA/AO(2D)	Left Atrium diameter/Aorta diameter	LA Diam (cm) / Ao Diam (cm)
AO/LA(2D)	Aorta diameter/Left Atrium diameter	Ao Diam (cm) / LA Diam (cm)

8.3.3.2 M Mode

The measurement items, calculation items and measurement method for M cardiology measurement are shown in the table below.

Table 31 M Cardiology Measurement

Items	Description	Methods or Formula
Ao Arch Diam(M)	Aorta Arch Diameter (M)	See "8.2.2.2 Distance (M)"
Ao Asc Diam(M)	Ascending Aorta Diameter (M)	See "8.2.2.2 Distance (M)"
Ao Desc Diam(M)	Descending Aorta Diameter (M)	See "8.2.2.2 Distance (M)"
Ao Diam(M)	Aorta Diameter (M)	See "8.2.2.2 Distance (M)"

Items	Description	Methods or Formula
Ao Isthmus(M)	Aorta Isthmus Diameter (M)	See “8.2.2.2 Distance (M)”
Ao Sinus Diam(M)	Aorta Sinus Diameter (M)	See “8.2.2.2 Distance (M)”
Ao st junct(M)	Aorta ST junct Diameter (M)	See “8.2.2.2 Distance (M)”
ACS(M)	Aortic Valve Cusp Separation (M)	See “8.2.2.2 Distance (M)”
HR(Cube M)	Heart Rate (Cube M)	See “0 M mode general measurement is applicable for general measurement of M images and anatomical M images. HR (M)”
HR(Gibson M)	Heart Rate (Cube M)	See “0 M mode general measurement is applicable for general measurement of M images and anatomical M images. HR (M)”
HR(Teich M)	Heart Rate (Cube M)	See “0 M mode general measurement is applicable for general measurement of M images and anatomical M images. HR (M)”
IVSd(M)	Interventricular Septal Thickness at end-diastole (M)	See “8.2.2.2 Distance (M)”
IVSs(M)	Interventricular Septal Thickness at end-systole (M)	See “8.2.2.2 Distance (M)”
LA Diam(M)	Left Atrium Diameter (M)	See “8.2.2.2 Distance (M)”
LPA Diam(M)	Left Pulmonary Artery Diameter (M)	See “8.2.2.2 Distance (M)”
Diastole(Cube M)	End-diastolic Left Ventricular Measurement (Cube 2D)	See “8.3.3.4 Cardiology Study and Calculation”
Diastole(Gibson M)	End-diastolic Left Ventricular Measurement (Gibson 2D)	See “8.3.3.4 Cardiology Study and Calculation”
Diastole(Teich M)	End-diastolic Left Ventricular Measurement (Teich 2D)	See “8.3.3.4 Cardiology Study and Calculation”
Systole(Cube M)	End-systolic Left Ventricular Measurement (Cube 2D)	See “8.3.3.4 Cardiology Study and Calculation”
Systole(Gibson M)	End-systolic Left Ventricular	See “8.3.3.4 Cardiology Study

Items	Description	Methods or Formula
	Measurement (Gibson 2D)	and Calculation"
Systole(Teich M)	End-systolic Left Ventricular Measurement (Teich 2D)	See "8.3.3.4 Cardiology Study and Calculation"
LVET(M)	Left Ventricular Ejection Time (M)	See "8.2.2.3 Time (M)"
LVIDd(Cube M)	Left Ventricular Internal Diameter at end-diastole (Cube M)	See "8.2.2.2 Distance (M)"
LVIDd(Gibson M)	Left Ventricular Internal Diameter at end-diastole (Gibson M)	See "8.2.2.2 Distance (M)"
LVIDd(Teich M)	Left Ventricular Internal Diameter at end-diastole (Teich M)	See "8.2.2.2 Distance (M)"
LVIDd(M)	Left Ventricular Internal Diameter at end-diastole (M)	See "8.2.2.2 Distance (M)"
LVIDs(M)	Left Ventricular Internal Diameter at end-systole (M)	See "8.2.2.2 Distance (M)"
LVIDs(Cube M)	Left Ventricular Internal Diameter at end-systole (Cube M)	See "8.2.2.2 Distance (M)"
LVIDs(Gibson M)	Left Ventricular Internal Diameter at end-systole (Gibson M)	See "8.2.2.2 Distance (M)"
LVIDs(Teich M)	Left Ventricular Internal Diameter at end-systole (Teich M)	See "8.2.2.2 Distance (M)"
LVPEP(M)	Left Ventricular Pre-Ejection Period (M)	See "8.2.2.3 Time (M)"
LVPWd(M)	Left Ventricular Posterior Wall Thickness at end-diastole (M)	See "8.2.2.2 Distance (M)"
LVPWs(M)	Left Ventricular Posterior Wall Thickness at end-systole (M)	See "8.2.2.2 Distance (M)"
MCS(M)	Mitral Valve Cusp Separation (M)	See "8.2.2.2 Distance (M)"
MPA Diam(M)	Main pulmonary Artery Diameter (M)	See "8.2.2.2 Distance (M)"
MV A Amp	Amplitude of the Mitral Valve A wave	See "8.2.2.2 Distance (M)"
MV E Amp	Amplitude of the Mitral Valve E wave	See "8.2.2.2 Distance (M)"
MV D-E Slope	Mitral Valve D-E Slope	See "8.2.2.4 Slope"
MV DE	Amplitude of the Mitral Valve DE wave	See "8.2.2.2 Distance (M)"
MV E-F Slope	Mitral Valve E-F Slope	See "8.2.2.4 Slope"
MV EPSS(M)	Distance between point E and Interventricular Septum when Mitral Valve is fully open (M)	See "8.2.2.2 Distance (M)"
PEd(M)	Pericardial Effusion at diastole (M)	See "8.2.2.2 Distance (M)"

Items	Description	Methods or Formula
PEs(M)	Pericardial Effusion at systole (M)	See “8.2.2.2 Distance (M)”
RPA Diam(M)	Right pulmonary Artery Diameter (M)	See “8.2.2.2 Distance (M)”
RVAWd(M)	Right Ventricular Anterior Wall Thickness at end-diastole (M)	See “8.2.2.2 Distance (M)”
RVAWs(M)	Right Ventricular Anterior Wall Thickness at end-systole (M)	See “8.2.2.2 Distance (M)”
RVDd(M)	Right Ventricular Diameter at end-diastole (M)	See “8.2.2.2 Distance (M)”
RVDs(M)	Right Ventricular Diameter at end-systole (M)	See “8.2.2.2 Distance (M)”
RVET(M)	Right Ventricular Ejection Time (M)	See “8.2.2.3 Time (M)”
RVPEP(M)	Right Ventricular Pre-Ejection Period (M)	See “8.2.2.3 Time (M)”
TAPSE	Tricuspid Annular Plane Systolic Excursion	See “8.2.2.2 Distance (M)”
IVSd(LV Mass Cube-M)	Interventricular Septal Thickness at end-diastole (LV Mass Cube-M)	See “8.2.2.2 Distance (M)”
LVIDd(LV Mass Cube-M)	Left Ventricular Internal Diameter at end-diastole (LV Mass Cube-M)	See “8.2.2.2 Distance (M)”
LVPWd(LV Mass Cube-M)	Left Ventricular Posterior Wall Thickness at end-diastole (LV Mass Cube-M)	See “8.2.2.2 Distance (M)”
MV C-O dur	Mitral Valve Close-Open Duration	See “8.2.2.3 Time (M)”
LVET(LV Tei Index-M)	Left Ventricular Ejection Time	See “8.3.3.4 Cardiology Study and Calculation”
LA/AO(M)	Left Atrium diameter/Aorta diameter (M)	LA Diam (cm) / Ao Diam (cm)
AO/LA(M)	Aorta diameter/Left Atrium diameter (M)	Ao Diam (cm) / LA Diam (cm)
MV ALL	Mitral Valve ALL	See “8.3.3.4 Cardiology Study and Calculation”

8.3.3.3 Doppler Mode

The measurement items, calculation items and measurement method for Doppler cardiology measurement are shown in the table below.

Table 32 Doppler Cardiology Measurement

Items	Description	Methods or Formula
MV Aa(lateral)	Mitral Valve medial Late diastolic motion	See “8.2.3.1 Vel”
MV Aa(medial)	Mitral Valve lateral Late diastolic motion	See “8.2.3.1 Vel”
AAo Vmax	Ascending Aorta Maximum Velocity	See “8.2.3.1 Vel”

Items	Description	Methods or Formula
AV VTI	Aorta Valve Velocity-Time Integral	See "8.2.3.5 D Trace"
AV Vmax	Aorta Valve Maximum Velocity	See "8.2.3.1 Vel"
AR DecT	Aortic Valve Regurgitation Deceleration Time	See "8.2.3.8 Acceleration"
AR PHT	Aortic Valve Regurgitation Pressure Half Time	See "8.3.3.4 Cardiology Study and Calculation"
AR Ved	Aortic Valve Regurgitation Velocity at end-diastole	See "8.2.3.1 Vel"
AR Vmax	Aortic Valve Regurgitation Maximum Velocity	See "8.2.3.1 Vel"
AR VTI	Aortic Valve Regurgitation Velocity-Time Integral	See "8.2.3.5 D Trace"
MV ARa(lateral)	Mitral Valve lateral Acceleration Rate	See "8.2.3.1 Vel"
MV ARa(medial)	Mitral Valve medial Acceleration Rate	See "8.2.3.1 Vel"
ASD Vmax	Atrial Septal Defect Maximum Velocity	See "8.2.3.1 Vel"
AV AccT	Aorta Valve Acceleration Time	See "8.2.3.3 Time (Doppler)"
AV DecT	Aorta Valve DecelerationTime	See "8.2.3.3 Time (Doppler)"
Coarc Pre-Duct	Coarctation of Pre-Ductus	See "8.2.3.1 Vel"
Coarc Post-Duct	Coarctation of Post-Ductus	See "8.2.3.1 Vel"
DAo Vmax	Descending Aorta Maximum Velocity	See "8.2.3.1 Vel"
MV DRa(lateral)	Mitral Valve lateral Deceleration Rate	See "8.2.3.1 Vel"
MV DRa(medial)	Mitral Valve medial Deceleration Rate	See "8.2.3.1 Vel"
MV Ea(lateral)	Mitral Valve lateral Early diastolic motion	See "8.2.3.1 Vel"
MV Ea(medial)	Mitral Valve medial Early diastolic motion	See "8.2.3.1 Vel"
HR(Doppler)	Heart Rate (Doppler)	See "8.2.3.4 HR (Doppler)"
IVC Vel(Expir)	Inferior Vena Cava Expiration Maximum Velocity	See "8.2.3.1 Vel"
IVC Vel(Insp)	Inferior Vena Cava Inspiration Maximum Velocity	See "8.2.3.1 Vel"
IVCT	Isovolumic Contraction Time	See "8.2.3.3 Time (Doppler)"

Items	Description	Methods or Formula
LPA Vmax	Left Pulmonary Artery Maximum Velocity	See “8.2.3.1 Vel”
LVET(D)	Left Ventricular Ejection Time (D)	See “8.2.3.3 Time (Doppler)”
LVOT AccT	Left Ventricular Outflow Tract Acceleration Time	See “8.2.3.3 Time (Doppler)”
LVOT VTI	Left Ventricular Outflow Tract Velocity-Time Integral	See “8.2.3.5 D Trace”
LVOT Vmax	Left Ventricular Outflow Tract Velocity	See “8.2.3.1 Vel”
LVPEP(D)	Left Ventricular Pre-ejection Period (D)	See “8.2.3.3 Time (Doppler)”
MPA Vmax	Main Pulmonary Artery Maximum Velocity	See “8.2.3.1 Vel”
dP/dt	Rate of Pressure change	/
MR VTI	Mitral Valve Regurgitation Velocity-Time Integral	See “8.2.3.5 D Trace”
MR Vmax	Mitral Valve Stenosis Maximum Velocity	See “8.2.3.1 Vel”
MS Vmax	Mitral Valve Stenosis Maximum Velocity	See “8.2.3.1 Vel”
MV A Dur	Mitral Valve A-wave Duration	See “8.2.3.3 Time (Doppler)”
MV A Vel	Mitral Valve A-wave Velocity	See “8.2.3.1 Vel”
MV A VTI	Mitral Valve A-wave Velocity-Time Integral	See “8.2.3.5 D Trace”
MV AccT	Mitral Valve Acceleration Time	See “8.2.3.3 Time (Doppler)”
MV DecT	Mitral Valve Deceleration Time	See “8.2.3.3 Time (Doppler)”
MV E Dur	Mitral Valve E-wave Duration	See “8.2.3.3 Time (Doppler)”
MV E Vel	Mitral Valve E-wave Velocity	See “8.2.3.1 Vel”
MV E VTI	Mitral Valve E-wave Velocity-Time Integral	See “8.2.3.5 D Trace”
IVRT	Isovelocity Relaxation Time	See “8.2.3.3 Time (Doppler)”
MV VTI	Mitral Valve Velocity-Time Integral	See “8.2.3.5 D Trace”
MV Vmax	Mitral Valve Maximum Velocity	See “8.2.3.1 Vel”
PVein A Dur	Pulmonary Vein A-wave Flow Duration	See “8.2.3.3 Time (Doppler)”
PVein A Vel	Pulmonary Vein A-wave Flow Velocity	See “8.2.3.1 Vel”
PVein D Vel	Pulmonary Vein D-wave Flow Velocity	See “8.2.3.1 Vel”

Items	Description	Methods or Formula
PVein D VTI	Pulmonary Vein D-wave Velocity-Time Integral	See "8.2.3.5 D Trace"
PVein DecT	Pulmonary Vein Deceleration Time	See "8.2.3.3 Time (Doppler)"
PVein S Vel	Pulmonary Vein S-wave Flow Velocity	See "8.2.3.1 Vel"
PVein S VTI	Pulmonary Vein S-wave Velocity-Time Integral	See "8.2.3.5 D Trace"
PDA Vel(d)	Patent Ductus Arteriosus Velocity at end-diastole	See "8.2.3.1 Vel"
PDA Vel(s)	Patent Ductus Arteriosus Velocity at end-systole	See "8.2.3.1 Vel"
PR PHT	Pulmonary Valve Regurgitation Pressure Half Time	See "8.3.3.4 Cardiology Study and Calculation"
PR VTI	Pulmonary Valve Regurgitation Velocity-Time Integral	See "8.2.3.5 D Trace"
PR Ved	Pulmonary Valve Regurgitation Velocity at end-diastole	See "8.2.3.1 Vel"
PR Vmax	Pulmonary Valve Regurgitation Maximum Velocity	See "8.2.3.1 Vel"
PV AccT	Pulmonary Valve Acceleration Time	See "8.2.3.3 Time (Doppler)"
PV VTI	Pulmonary Valve Velocity-Time Integral	See "8.2.3.5 D Trace"
PV Vmax	Pulmonary Valve Maximum Velocity	See "8.2.3.1 Vel"
RAP	Right Atrium Pressure	/
RPA Vmax	Right Pulmonary Artery Maximum Velocity	See "8.2.3.1 Vel"
RVET(D)	Right Ventricular Ejection Time (D)	See "8.2.3.3 Time (Doppler)"
RVOT Vmax	Right Ventricular Outflow Tract Maximum Velocity	See "8.2.3.1 Vel"
ROVT VTI	Right Ventricular Outflow Tract Velocity-Time Integral	See "8.2.3.5 D Trace"
RVPEP(D)	Right Ventricular Pre-Ejection Period (D)	See "8.2.3.3 Time (Doppler)"
MV Sa(lateral)	Mitral Valve lateral Systolic motion	See "8.2.3.1 Vel"
MV Sa(medial)	Mitral Valve medial Systolic motion	See "8.2.3.1 Vel"
SVC Vel(Expir)	Superior Vena Cava Expiration Maximum Velocity	See "8.2.3.1 Vel"

Items	Description	Methods or Formula
SVC Vel(Insp)	Superior Vena Cava Inspiration Maximum Velocity	See “8.2.3.1 Vel”
TR VTI	Tricuspid Valve Regurgitation Velocity-Time Integral	See “8.2.3.5 D Trace”
TR Vmax	Tricuspid Valve Regurgitation Maximum Velocity	See “8.2.3.1 Vel”
TV A Dur	Tricuspid Valve A-wave Duration	See “8.2.3.3 Time (Doppler)”
TV A Vel	Tricuspid Valve A-wave Flow Velocity	See “8.2.3.1 Vel”
TV AccT	Tricuspid Valve Acceleration Time	See “8.2.3.3 Time (Doppler)”
TV DecT	Tricuspid Valve Deceleration Time	See “8.2.3.3 Time (Doppler)”
TV E Vel	Tricuspid Valve E-wave Flow Velocity	See “8.2.3.1 Vel”
TV VTI	Tricuspid Valve Velocity-Time Integral	See “8.2.3.5 D Trace”
TV Vmax	Tricuspid Valve Maximum Velocity	See “8.2.3.1 Vel”
VSD Vmax	Ventricular Septal Defect Maximum Velocity	See “8.2.3.1 Vel”
Hepatic V S Vel	Hepatic Vein Systolic Peak Velocity	See “8.2.3.1 Vel”
Hepatic V D Vel	Hepatic Vein Diastolic Peak Velocity	See “8.2.3.1 Vel”
MV HR	Mitral Valve Heart Rate	See “8.2.3.4 HR (Doppler)”
TV HR	Tricuspid valve Heart Rate	See “8.2.3.4 HR (Doppler)”
PV HR	Pulmonary Valve Heart Rate	See “8.2.3.4 HR (Doppler)”
MV C-O dur(D)	Mitral Valve close-open Duration (D)	See “8.2.3.3 Time (Doppler)”
LVET(LV Tei Index-Doppler)	Left Ventricular Ejection Time	See “8.3.3.4 Cardiology Study and Calculation”
AR Rad	Aortic Valve Stenosis Radius	See “8.3.3.4 Cardiology Study and Calculation”
AR Als Vel	Aortic Valve Regurgitation Aliasing Maximum Velocity	See “8.3.3.4 Cardiology Study and Calculation”
MR Rad	Mitral Valve Stenosis Radius	See “8.3.3.4 Cardiology Study and Calculation”
MR Als Vel	Mitral Valve Regurgitation Aliasing Maximum Velocity	See “8.3.3.4 Cardiology Study and Calculation”

Items	Description	Methods or Formula
PR Rad	Pulmonary Valve Stenosis Radius	See “8.3.3.4 Cardiology Study and Calculation”
PR Als Vel	Pulmonary Valve Regurgitation Aliasing Maximum Velocity	See “8.3.3.4 Cardiology Study and Calculation”
TR Rad	Tricuspid Valve Stenosis Radius	See “8.3.3.4 Cardiology Study and Calculation”
TR Als Vel	Tricuspid Valve Regurgitation Aliasing Maximum Velocity	See “8.3.3.4 Cardiology Study and Calculation”
TV C-O dur	Tricuspid Valve close-open Duration	See “8.2.3.3 Time (Doppler)”
RVET(RV Tei Index)	Right Ventricular Ejection Time	See “8.2.3.3 Time (Doppler)”
MV E/A	Mitral Valve E-Vel/A-Vel	See “8.3.3.4 Cardiology Study and Calculation”
MVA(PHT)	Mitral Valve Orifice Area (PHT)	See “8.3.3.4 Cardiology Study and Calculation”
TV E/A	Tricuspid Valve E-Vel/A-Vel	See “8.3.3.4 Cardiology Study and Calculation”
TVA(PHT)	Tricuspid Valve Orifice Area (PHT)	See “8.3.3.4 Cardiology Study and Calculation”

8.3.3.4 Cardiology Study and Calculation

➤ Simpson SP

Measurement and study	Description	Method and Formula
EDV(Simp SP)	End-diastolic Left Ventricular Volume	$EDV(ml) = \pi \times \frac{LVLd\ apical(cm)}{20} \times \sum_{i=1}^{20} r_i^2\ (cm)$ LVLd apical: left Ventricular Long-axis Length at End-diastole in apical view r_i: radius measured during diastole
ESV(Simp SP)	End-systolic Left Ventricular Volume	$ESV(ml) = \pi \times \frac{LVLs\ apical(cm)}{20} \times \sum_{i=1}^{20} r_i^2\ (cm)$ LVLs apical: left Ventricular Long-axis

Measurement and study	Description	Method and Formula
		Length at End-systole in apical view r_i : radius measured during systole
EDV Index (Simp SP)	/	EDV Index=EDV/BSA
ESV Index (Simp SP)	/	ESV Index=ESV/BSA
SV	Stroke Volume	SV(ml) = EDV(ml)-ESV(ml)
CO	Cardiac Output	CO(l/min) = SV(ml)×HR(bpm)/ 1000
EF	Ejection Fraction	EF(No unit) = SV(ml)/ EDV(ml)
SI	SV Index	SI(No unit) = SV(ml)/ Body Surface Area (m ²)
CI	CO Index	CI(No unit) = CO(l/min)/Body Surface Area (m ²)

➤ **Simpson BP**

Measurement and study	Description	Method and Formula
EDV(Simpson BP)	End-diastolic Left Ventricular Volume	*1
ESV(Simpson BP)	End-systolic Left Ventricular Volume	*2
EDV Index (Simpson BP)	/	EDV Index=EDV/BSA
ESV Index (Simpson BP)	/	ESV Index=ESV/BSA
SV(Simpson BP)	Stroke Volume	SV(ml) = EDV(ml)-ESV(ml)
CO(Simpson BP)	Cardiac Output	CO(l/min) = SV(ml)×HR(bpm)/ 1000
EF(Simpson BP)	Ejection Fraction	EF(No unit) = SV(ml)/ EDV(ml)
SI(Simpson BP)	SV Index	SI(No unit) = SV(ml)/ Body Surface Area (m ²)
CI(Simpson BP)	CO Index	CI(No unit) = CO(l/min)/Body Surface Area (m ²)

➤ ***1 Means:**

$$EDV(ml) = \pi \times \frac{MAX\{LV Ld_{2i}(cm), LV Ld_{4i}(cm)\}}{20} \times \sum_{i=1}^{20} (r_{2i}(cm) \times r_{4i}(cm))$$

➤ ***2 Means:**

$$ESV(ml) = \pi \times \frac{MAX\{LVLS_{2i}(cm), LVLS_{4i}(cm)\}}{20} \times \sum_{i=1}^{20} (r_{2i}(cm) \times r_{4i}(cm))$$

➤ **LV volume (A2C):**

$$EDV (2ml) = \pi \times \frac{LVLD_{2i}(cm)}{20} \times \sum_{i=1}^{20} r_{2i}^2 (cm)$$

$$ESV (2ml) = \pi \times \frac{LVLS_{2i}(cm)}{20} \times \sum_{i=1}^{20} r_{2i}^2 (cm)$$

➤ **LV volume (A4C):**

$$EDV (4ml) = \pi \times \frac{LVLD_{4i}(cm)}{20} \times \sum_{i=1}^{20} r_{4i}^2 (cm)$$

$$ESV (4ml) = \pi \times \frac{LVLS_{4i}(cm)}{20} \times \sum_{i=1}^{20} r_{4i}^2 (cm)$$

NOTE: When using Simpson BP to measure LV function, be sure to keep the apical four-chamber view and apical two-chamber view perpendicular. Otherwise the measure result will be incorrect.

➤ **Cube**

Measurement and study	Description	Method and Formula
Diastole	End-diastolic Left Ventricular Measurement	FoldLine in 2D mode or Parallel method in M mode
Systole	End-systolic Left Ventricular Measurement	FoldLine in 2D mode or Parallel method in M mode
LVIDd	Left Ventricular Internal Diameter at End-diastole	Distance in 2D/M General Measurements
LVIDs	Left Ventricular Internal Diameter at End-systole	Distance in 2D/M General Measurements
HR	Heart Rate	Obtained by ECG, input directly or measure manually
IVSd	Interventricular Septal Thickness at End-diastole	Distance in 2D/M General Measurements
LVPWd	Left Ventricular Posterior Wall Thickness at End-diastole	Distance in 2D/M General Measurements

Measurement and study	Description	Method and Formula
EDV(Cube)	End-diastolic Left Ventricular Volume	$EDV(ml) = LVIDd(cm)^3$
ESV(Cube)	End-systolic Left Ventricular Volume	$ESV(ml) = LVIDs(cm)^3$
EDV Index (Cube)	/	$EDV\ Index = EDV/BSA$
ESV Index (Cube)	/	$ESV\ Index = ESV/BSA$
SV (Cube)	Stroke Volume	$SV(ml) = EDV(ml) - ESV(ml)$
CO (Cube)	Cardiac Output	$CO(l/min) = SV(ml) \times HR(bpm) / 1000$
EF (Cube)	Ejection Fraction	$EF(No\ unit) = SV(ml) / EDV(ml)$
SI (Cube)	SV Index	$SI(No\ unit) = SV(ml) / Body\ Surface\ Area\ (m^2)$
CI (Cube)	CO Index	$CI(No\ unit) = CO(l/min) / Body\ Surface\ Area\ (m^2)$

➤ **Teichholz**

Measurement and study	Description	Method and Formula
Diastole	End-diastolic Left Ventricular Measurement	FoldLine in 2D mode or Parallel method in M mode
Systole	End-systolic Left Ventricular Measurement	FoldLine in 2D mode or Parallel method in M mode
LVIDd	Left Ventricular Internal Diameter at End-diastole	Distance in 2D/M General Measurements
LVIDs	Left Ventricular Internal Diameter at End-systole	Distance in 2D/M General Measurements
HR	Heart Rate	Obtained by ECG, input directly or measure manually
IVSd	Interventricular Septal Thickness at End-diastole	Distance in 2D/M General Measurements
LVPWd	Left Ventricular Posterior Wall Thickness at End-diastole	Distance in 2D/M General Measurements
IVSs	Interventricular Septal Thickness at End-systole	Distance in 2D/M General Measurements

Measurement and study	Description	Method and Formula
LVPWs	Left Ventricular Posterior Wall Thickness at End-systole	Distance in 2D/M General Measurements
EDV(Teichholz)	End-diastolic Left Ventricular Volume	$EDV(ml) = (7 \times (LVIDd(cm))^3) / (2.4 + LVIDd(cm))$
ESV(Teichholz)	End-systolic Left Ventricular Volume	$ESV(ml) = (7 \times (LVIDs(cm))^3) / (2.4 + LVIDs(cm))$
SV (Teichholz)	Stroke Volume	$SV(ml) = EDV(ml) - ESV(ml)$
CO (Teichholz)	Cardiac Output	$CO(l/min) = SV(ml) \times HR(bpm) / 1000$
EF (Teichholz)	Ejection Fraction	$EF(\text{No unit}) = SV(ml) / EDV(ml)$
FS (Teichholz)	Fractional Shortening	$FS(\text{No unit}) = (LVIDd(cm) - LVIDs(cm)) / LVIDd(cm)$
MVCF (Teichholz)	Mean Velocity of Circumferential Fiber Shortening	$MVCF = (LVIDd(cm) - LVIDs(cm)) / (LVIDd(cm) \times LVET(s))$
SI (Teichholz)	SV Index	$SI(\text{No unit}) = SV(ml) / \text{Body Surface Area (m}^2\text{)}$
CI (Teichholz)	CO Index	$CI(\text{No unit}) = CO(l/min) / \text{Body Surface Area (m}^2\text{)}$

➤ **Gibson**

Measurement and study	Description	Method and Formula
Diastole	End-diastolic Left Ventricular Measurement	FoldLine in 2D mode or Parallel method in M mode
Systole	End-systolic Left Ventricular Measurement	FoldLine in 2D mode or Parallel method in M mode
LVIDd	Left Ventricular Internal Diameter at End-diastole	Distance in 2D/M General Measurements
LVIDs	Left Ventricular Internal Diameter at End-systole	Distance in 2D/M General Measurements
HR	Heart Rate	Obtained by ECG, input directly or measure manually
IVSd	Interventricular Septal Thickness at End-diastole	Distance in 2D/M General Measurements

Measurement and study	Description	Method and Formula
LVPWd	Left Ventricular Posterior Wall Thickness at End-diastole	Distance in 2D/M General Measurements
IVSs	Interventricular Septal Thickness at End-systole	Distance in 2D/M General Measurements
LVPWs	Left Ventricular Posterior Wall Thickness at End-systole	Distance in 2D/M General Measurements
EDV(Gibson)	End-diastolic Left Ventricular Volume	$EDV(ml) = \pi/6(0.98 \times LVIDd(cm) + 5.90) \times LVIDd(cm)^2$
ESV(Gibson)	End-systolic Left Ventricular Volume	$ESV(ml) = \pi/6(1.14 \times LVIDs(cm) + 4.18) \times LVIDs(cm)^2$
EDV Index (Gibson)	/	EDV Index=EDV/BSA
ESV Index (Gibson)	/	ESV Index=ESV/BSA
SV (Gibson)	Stroke Volume	$SV(ml) = EDV(ml) - ESV(ml)$
CO (Gibson)	Cardiac Output	$CO(l/min) = SV(ml) \times HR(bpm) / 1000$
EF (Gibson)	Ejection Fraction	$EF(\text{No unit}) = SV(ml) / EDV(ml)$
FS (Gibson)	Fractional Shortening	$FS(\text{No unit}) = (LVIDd(cm) - LVIDs(cm)) / LVIDd(cm)$
MVCF (Gibson)	Mean Velocity of Circumferential Fiber Shortening	$MVCF = (LVIDd(cm) - LVIDs(cm)) / (LVIDd(cm) \times EF(s))$
SI (Gibson)	SV Index	$SI(\text{No unit}) = SV(ml) / \text{Body Surface Area (m}^2\text{)}$
CI (Gibson)	CO Index	$CI(\text{No unit}) = CO(l/min) / \text{Body Surface Area (m}^2\text{)}$

➤ LV Mass

Estimate the Index of Left Ventricular Mass (LV Mass-I) by calculating the LV Mass.

LV Mass (Cube)

Measurement and study	Description	Method and Formula
IVSd	Interventricular Septal Thickness at End-diastole	Distance in 2D/M General Measurements
LVIDd	Left Ventricular Internal Diameter at End-diastole	Distance in 2D/M General Measurements
LVPWd	Left Ventricular Posterior Wall Thickness at End-diastole	Distance in 2D/M General Measurements
LV Mass (Cube)	Left Ventricular Mass	*1

Measurement and study	Description	Method and Formula
LV MASS-I (Cube)	Index of Left Ventricular Mass	*2

*1 Means:

$$LV\ Mass(g) = 1.04 \times ((LVPWd(cm) + IVSd(cm) + LVIdDd(cm))^3 - LVId(cm)^3) - 13.6$$

*2 Means:

$$LV\ Mass-I\ (No\ unit) = LV\ Mass\ (g) / Body\ Surface\ Area\ (m^2)$$

LV Mass (A-L)

Measurement and study	Description	Method and Formula
LVAd sax Epi	Left Ventricular Epicardial Area at Papillary Muscle level at end-diastole in Short-axis view	Area in 2D/M General Measurements
LVAd sax Endo	Left Ventricular Endocardial Area at Papillary Muscle level at end-diastole in Short-axis view	Area in 2D/M General Measurements
LVLd apical	Left Ventricular Long-axis Length at End-diastole in apical view	Distance in 2D/M General Measurements
LV Mass (A-L)	Left Ventricular Mass	*1
LV MASS-I (A-L)	Index of Left Ventricular Mass	*2

*1 Means:

$$LV\ Mass(g) = 1.05 \times 5/6 \times (LVAd\ sax\ Epi(cm^2) \times (LVLd\ apical(cm) + t(cm)) - LVAd\ sax\ Endo(cm^2) \times LVL(cm));$$

$$t(cm) = \sqrt{\left(\frac{LVAd\ sax\ Epi(cm^2)}{\pi}\right)} - \sqrt{\left(\frac{LVAd\ sax\ Endo(cm^2)}{\pi}\right)}$$

*2 Means:

$$LV\ Mass-I\ (No\ unit) = LV\ Mass\ (g) / Body\ Surface\ Area\ (m^2)$$

LV Mass (T-E)

Measurement and study	Description	Method and Formula
LVAd sax Epi	Left Ventricular Epicardial Area at Papillary Muscle level at end-diastole in Short-axis view	Area in 2D General Measurements

Measurement and study	Description	Method and Formula
LVAd sax Endo	Left Ventricular Endocardial Area atPapillary Muscle level at end-diastole in Short-axisview	Area in 2D General Measurements
a	Semi-major axis from widest minor axis radius to apex	Distance in 2D General Measurements
b	Truncated semi-major axis from widest minor axis radius to mitral annulus plane	Distance in 2D General Measurements
LV Mass (T-E)	Left Ventricular Mass	*1
LV MASS-I (T-E)	Index of Left Ventricular Mass	*2

*1 Means:

$$LV\ Mass(g) = 1.05\pi \times \left\{ (b+t)^2 \times \left[\frac{2(a+t)}{3} + d - \frac{d^3}{3(a+t)^2} \right] - b^2 \times \left(\frac{2a}{3} + d - \frac{d^3}{3a^2} \right) \right\}$$

$$t(cm) = \sqrt{\left(\frac{LVAdsaxEpi(cm^2)}{\pi} \right)} - \sqrt{\left(\frac{LVAdsaxEndo(cm^2)}{\pi} \right)}$$

$$b(cm) = \sqrt{\frac{LVAdsaxEndo(cm^2)}{\pi}}$$

*2 Means:

$$LV\ Mass-I\ (No\ unit) = LV\ Mass\ (g) / Body\ Surface\ Area\ (m^2)$$

➤ Mitral Valve Area (MVA)

Mitral Valve Area (MVA) can be calculated by two methods: pressure half time (PHT) or velocity- time integral (VTI).

MVA (VTI)

Measurement and study	Description	Method and Formula
LVOT Diam	Left Ventricular Outflow Tract Diameter	Distance in 2D General Measurements
LVOT VTI	Left Ventricular Outflow Tract Velocity-Time Integral	D trace in Doppler General Measurement
MV VTI	Mitral Valve Velocity-Time Integral	D trace in Doppler General Measurement
MVA(VTI)	Mitral Valve Area	*1

*1 Means:

$$MVA(VTI)(cm^2) = \frac{\pi \times |LVOT\ VTI(cm)| \times LVOT\ Diam(cm)^2}{4 \times |MV\ VTI(cm)|}$$

➤ **AVA (VTI)**

Aortic Valve Area (AVA) can be calculated by velocity-time integral (VTI).

Measurement and study	Description	Method and Formula
LVOT Diam	Left Ventricular Outflow Tract Diameter	Distance in 2D General Measurements
LVOT VTI	Left Ventricular Outflow Tract Velocity-Time Integral	D trace in Doppler General measurements
AV VTI	Aortic Valve Velocity-Time Integral	D trace in Doppler General measurements
AVA(VTI)	Aortic Valve Area	*1

*1 Means:

$$AVA(VTI)(cm^2) = \frac{\pi \times |LVOT VTI(cm)| \times LVOT Diam(cm)^2}{4 \times |AV VTI(cm)|}$$

➤ **LA Vol**

LA Vol (A-L)

Measurement and study	Description	Method and Formula
LA Diam	Left Atrium Diameter	Distance in 2D General Measurements
LAA(A2C)	Left Atrium Area at apical 2-chamber view	Area in 2D General Measurements
LAA(A4C)	Left Atrium Area at apical 4-chamber view	Area in 2D General Measurements
LA Vol(A-L)	Left Atrium Area	*1

*1 Means:

$$LA Vol(A-L)(ml) = \frac{8\pi}{3} LAA(A4C)(cm^2) \times LAA(A2C)(cm^2) / LA Diam(cm)$$

LA Vol (Simp)

Measurement and study	Description	Method and Formula
LA Vol(A2C)	Left Atrium Volume at apical 2-chamber view	Same as Simpson SP measurement
LA Vol(A4C)	Left Atrium Volume at apical 4-chamber view	Same as Simpson SP measurement

➤ **RA Vol (Simp)**

Measurement and study	Description	Method and Formula
RA Vol(A4C)	Right Atrium Volume at apical 4-chamber view	Same as Simpson SP measurement

➤ **LVIMP**

Measurement and study	Description	Method and Formula
MV C-O dur	Mitral Valve close-open Duration	Time in M/Doppler General Measurements
LVET	Left Ventricular Ejection Time	Time in M/Doppler General Measurements
LVIMP	Left Ventricular Index of Myocardial Performance	*1

*1 Means:

$$LVIMP(no\ unit) = \frac{MV\ C-O\ dur(s) - LVET(s)}{LVET(s)}$$

➤ **RVSP**

Measurement and study	Description	Method and Formula
TR Vmax	Tricuspid Valve Regurgitation Maximum Velocity	D Vel in Doppler General Measurements
RAP	Right Atrium Pressure	Enter manually
TR PGmax	Tricuspid Valve Regurgitation Pressure Gradient	*1
RVSP	Right Ventricular Systolic Pressure	*2

*1 Means:

$$TR\ PGmax(mmHg) = 4 \times TR\ Vmax\ (m/s)^2$$

*2 Means:

$$RVSP(mmHg) = RAP(mmHg) + 4 \times (TR\ V\ max(m/s))^2$$

➤ **PAEDP**

Measurement and study	Description	Method and Formula
PR Ved	Pulmonary Valve Regurgitation Velocity at end-Diastole	D Vel in Doppler General Measurements
RAP	Right Atrium Pressure	Enter manually

Measurement and study	Description	Method and Formula
PR PGed	Pulmonary Valve Regurgitation Pressure Gradient at end-Diastole	/
PAEDP	Pulmonary Pressure at end-Diastole	*1

*1 Means:

$$PAEDP(\text{mmHg}) = RAP(\text{mmHg}) + 4 \times (PR.Ved \text{ (m/s)})^2$$

➤ **RV Tei index(RVIMP)**

Measurement and study	Description	Method and Formula
TV C-O dur	Tricuspid Valve close-open Duration	Time in Doppler General Measurements
RVET	Right Ventricular Ejection Time	Time in Doppler General Measurements
RVIMP	Right Ventricular Index of Myocardial Performance	*1

*1 Means:

$$RVIMP(\text{no unit}) = \frac{TV \text{ C-O dur}(s) - RVET(s)}{RVET(s)}$$

➤ **LV Tei index(LVIMP)**

Measurement and study	Description	Method and Formula
MV C-O dur	Mitral Valve close-open Duration	Time in Doppler General Measurements
LVET	Left Ventricular Ejection Time	Time in Doppler General Measurements
LVIMP	Left Ventricular Index of Myocardial Performance	*1

*1 Means:

$$LVIMP(\text{no unit}) = \frac{MV \text{ C-O dur}(s) - LVET(s)}{LVET(s)}$$

➤ **PISA**

PISA (Proximal Isovelocity Surface Area) is used in quantitative analysis of the mitral valve regurgitation (PISA MR), aortic valve regurgitation (PISA AR), tricuspid valve regurgitation (PISA TR), and pulmonary valve regurgitation (PISA PR) in color mode.

PISA MR

NOTE: Only applicable for Color and Doppler modes.

Measurement and study	Description	Method and Formula
MR Rad	Mitral Valve Stenosis Radius	PISA measurement
MR VTI	Mitral Valve Regurgitation Velocity-Time Integral	D Trace in Doppler General Measurements
MR Als.Vel	Mitral Valve Regurgitation Aliasing Maximum Velocity	You can select to use top aliasing velocity or bottom aliasing velocity or input the value directly.
MR Vmax	Mitral Regurgitation Maximum Velocity	Obtained from MR VTI measurement
MR Flow	Mitral Regurgitation Flow	*1
MR Flow Rate	Mitral Regurgitation Flow Rate	*2
MR Fraction	Mitral Valve Regurgitation Fraction	*3
MR EROA	Mitral Valve Effective Regurgitant Orifice Area	*4

*1 Means:

$$MR\ Flow(ml) = \frac{2\pi MR\ Rad(cm)^2 \times MR\ Als.Vel(cm/s)}{|MRV\ max\ (cm/s)|} \times |MR\ VTI(cm)|$$

*2 Means:

$$MR\ Flow\ Rate(ml/s) = 2\pi\ MR\ Rad(cm)^2 \times MR\ Als.Vel(cm/s)$$

*3 Means:

$$MR\ Fraction\ (no\ unit) = \frac{MR\ Flow(ml)}{MV\ SV(ml)} \times 100\%$$

*4 Means:

$$MR\ EROA(cm)^2 = \frac{2\pi MR\ Rad(cm)^2 \times MR\ Als.Vel(cm/s)}{|MR\ Vmax(cm/s)|}$$

PISA AR

NOTE: Only applicable for Color and Doppler modes.

Measurement and study	Description	Method and Formula
AR Rad	Aortic Valve Stenosis Radius	PISA measurement

AR VTI	Aortic Valve Regurgitation Velocity-Time Integral	D Trace in Doppler General Measurements
AR Als.Vel	Aortic Valve Regurgitation Aliasing Maximum Velocity	You can select to use top aliasing velocity or bottom aliasing velocity or input the value directly.
AR Vmax	Aortic Regurgitation Maximum Velocity	Obtained from AR VTI measurement
AR Flow	Aortic Regurgitation Flow	*1
AR Flow Rate	Aortic Regurgitation Flow Rate	*2
AR Fraction	Aortic Valve Regurgitation Fraction	*3
AR EROA	Aortic Valve Effective Regurgitant Orifice Area	*4

*1 Means:

$$AR\ Flow(ml) = \frac{2\pi AR\ Rad(cm)^2 \times AR\ Als.Vel(cm/s)}{|ARV\ max\ (cm/s)|} \times |AR\ VTI(cm)|$$

*2 Means:

$$AR\ Flow\ Rate(ml/s) = 2\pi\ AR\ Rad(cm)^2 \times AR\ Als.Vel(cm/s)$$

*3 Means:

$$AR\ Fraction\ (no\ unit) = \frac{AR\ Flow(ml)}{AV\ SV(ml)} \times 100\%$$

*4 Means:

$$AR\ EROA(cm)^2 = \frac{2\pi AR\ Rad(cm)^2 \times A\ Als.Vel(cm/s)}{|AR\ Vmax(cm/s)|}$$

PISA TR

NOTE: Only applicable for Color and Doppler modes.

Measurement and study	Description	Method and Formula
TR Rad	Tricuspid Valve Stenosis Radius	PISA measurement
TR VTI	Tricuspid Valve Regurgitation Velocity-Time Integral	D Trace in Doppler General Measurements
TR Als.Vel	Tricuspid Valve Regurgitation Aliasing Maximum Velocity	You can select to use top aliasing velocity or bottom aliasing velocity or input the value directly.

TR Vmax	Tricuspid Regurgitation Maximum Velocity	Obtained from TR VTI measurement
TR Flow	Tricuspid Regurgitation Flow	*1
TR Flow Rate	Tricuspid Regurgitation Flow Rate	*2
TR Fraction	Tricuspid Valve Regurgitation Fraction	*3
TR EROA	Tricuspid Valve Effective Regurgitant Orifice Area	*4

*1 Means:

$$TR\ Flow(ml) = \frac{2\pi TR\ Rad(cm)^2 \times TR\ Als.Vel(cm/s)}{|TRV\ max\ (cm/s)|} \times |TR\ VTI(cm)|$$

*2 Means:

$$TR\ Flow\ Rate(ml/s) = 2\pi\ TR\ Rad(cm)^2 \times TR\ Als.Vel(cm/s)$$

*3 Means:

$$TR\ Fraction\ (no\ unit) = \frac{TR\ Flow(ml)}{TV\ SV(ml)} \times 100\%$$

*4 Means:

$$TR\ EROA(cm)^2 = \frac{2\pi TR\ Rad(cm)^2 \times TR\ Als.Vel(cm/s)}{|TR\ Vmax(cm/s)|}$$

PISA PR

NOTE: Only applicable for Color and Doppler modes.

Measurement and study	Description	Method and Formula
PR Rad	Pulmonary Valve Stenosis Radius	PISA measurement
PR VTI	Pulmonary Valve Regurgitation Velocity-Time Integral	D Trace in Doppler General Measurements
PR Als.Vel	Pulmonary Valve Regurgitation Aliasing Maximum Velocity	You can select to use top aliasing velocity or bottom aliasing velocity or input the value directly.
PR Vmax	Pulmonary Regurgitation Maximum Velocity	Obtained from PR VTI measurement
PR Flow	Pulmonary Regurgitation Flow	*1
PR Flow Rate	Pulmonary Regurgitation Flow Rate	*2
PR Fraction	Pulmonary Valve Regurgitation Fraction	*3
PR EROA	Pulmonary Valve Effective	*4

	Regurgitant Orifice Area	
--	--------------------------	--

*1 Means:

$$PR\ Flow(ml) = \frac{2\pi PR\ Rad(cm)^2 \times PR\ Als.Vel(cm/s)}{|PRV\ max\ (cm/s)|} \times |PR\ VTI(cm)|$$

*2 Means:

$$PR\ Flow\ Rate(ml/s) = 2\pi PR\ Rad(cm)^2 \times PR\ Als.Vel(cm/s)$$

*3 Means:

$$PR\ Fraction\ (no\ unit) = \frac{PR\ Flow(ml)}{PV\ SV(ml)} \times 100\%$$

*4 Means:

$$PR\ EROA(cm)^2 = \frac{2\pi PR\ Rad(cm)^2 \times PR\ Als.Vel(cm/s)}{|PR\ Vmax(cm/s)|}$$

➤ TDI

Measurement and study	Description	Method and Formula
Ea/Aa(medial)	MV medial E-Vel/ A-Vel	$Ea / Aa(medial)(no\ unit) = \frac{Ea(medial)}{Aa(medial)}$
ATa(medial)	MV medial E-wave Acceleration Time	Obtained from ARa(medial) measurements
DTa(medial)	MV medial E-wave Deceleration Time	Obtained from DRa(medial) measurements
Ea/Aa(lateral)	MV lateral E-Vel/ A-Vel	$Ea / Aa(lateral)(no\ unit) = \frac{Ea(lateral)}{Aa(lateral)}$
ATa(lateral)	MV lateral E-wave Acceleration Time	Obtained from ARa(lateral) measurement
DTa(lateral)	MV lateral E-wave Deceleration Time	Obtained from DRa(lateral) measurement

➤ MV ALL

Measurement and study	Method and Formula
MV E Amp	See "8.2.2.2 Distance (M)"
MV D-E Amp	See "8.2.2.2 Distance (M)"
MV D-E Slope	See "8.2.2.4 Slope"
MV E-F Slope	See "8.2.2.4 Slope"
MV A Amp	See "8.2.2.2 Distance (M)"

MV A-C Interval	See “8.2.2.3 Time (M)”
-----------------	------------------------

8.3.4 Small Parts

8.3.4.1 2D Mode

The measurement items, calculation items and measurement method for 2D small parts measurement are shown in the table below.

Table 33 2D Small Parts Measurement

Items	Description	Methods or Formula
Thyroid L	Thyroid Length	See “8.2.1.1 Distance (2D)”
Thyroid H	Thyroid Height	See “8.2.1.1 Distance (2D)”
Thyroid W	Thyroid Width	See “8.2.1.1 Distance (2D)”
Isthmus H	Isthmus Height	See “8.2.1.1 Distance (2D)”
Testicular L	Testicular Length	See “8.2.1.1 Distance (2D)”
Testicular H	Testicular Height	See “8.2.1.1 Distance (2D)”
Testicular W	Testicular Width	See “8.2.1.1 Distance (2D)”
Testicular Mass1 d1-3	Testicular Mass diameter1	See “8.2.1.1 Distance (2D)”
Testicular Mass2 d1-3	Testicular Mass diameter2	See “8.2.1.1 Distance (2D)”
Testicular Mass3 d1-3	Testicular Mass diameter3	See “8.2.1.1 Distance (2D)”
Epididymis L	Epididymis Length	See “8.2.1.1 Distance (2D)”
Epididymis W	Epididymis Width	See “8.2.1.1 Distance (2D)”
Epididymis H	Epididymis Height	See “8.2.1.1 Distance (2D)”
Scrotal Wall	Scrotal Wall Thickness	See “8.2.1.1 Distance (2D)”
Breast Mass 1-10 L	Breast Mass Length	See “8.2.1.1 Distance (2D)”
Breast Mass 1-10 W	Breast Mass Height	See “8.2.1.1 Distance (2D)”
Breast Mass 1-10 H	Breast Mass Width	See “8.2.1.1 Distance (2D)”
Nip.-Mass 1~10 Dist.	Distance between nipple and mass	See “8.2.1.1 Distance (2D)”
Skin-Mass 1~10 Dist.	Distance between skin and mass	See “8.2.1.1 Distance (2D)”
Thyroid Mass 1~3 d1	Thyroid Mass diameter1	See “8.2.1.1 Distance (2D)”
Thyroid Mass 1~3 d2	Thyroid Mass diameter2	See “8.2.1.1 Distance (2D)”

Items	Description	Methods or Formula
Thyroid Mass 1~3 d3	Thyroid Mass diameter3	See “8.2.1.1 Distance (2D)”

8.3.4.2 Doppler Mode

Items	Description	Methods or Formula
SAT	Superior Thyroid Artery	See “8.2.3.5 D Trace”
ITA	Inferior Thyroid Artery	See “8.2.3.5 D Trace”
Testis A	Testis Artery	See “8.2.3.5 D Trace”
Testis V	Testis Vein	See “8.2.3.5 D Trace”
Epididymis A	Epididymis Artery	See “8.2.3.5 D Trace”
Epididymis V	Epididymis Vein	See “8.2.3.5 D Trace”

8.3.4.3 Little Parts Study and Calculation

Items	Description	Methods or Formula
Thyroid Vol	Thyroid Volume	Measure Thyroid L, Thyroid W and Thyroid H, system then automatically calculates the Thyroid Vol.
Testicular Vol	Testicular Volume	Measure Testicular L, Testicular W and Testicular H, system then automatically calculates the Thyroid Vol.

8.3.5 Vascular

8.3.5.1 2D Vascular Measurement

Table 34 2D Vascular Measurement

Items		Methods or Formula
IMT	CCA IMT	See “8.3.5.3 Vascular Study and Calculation”
	Bulb IMT	See “8.3.5.3 Vascular Study and Calculation”
	ICA IMT	See “8.3.5.3 Vascular Study and Calculation”
	ECA IMT	See “8.3.5.3 Vascular Study and Calculation”
CCA	Outer Diameter	See “8.2.1.1 Distance (2D)”
	Inner Diameter	See “8.2.1.1 Distance (2D)”
	Outer Area	See “8.2.1.2 Area & Circumference”
	Inner Area	See “8.2.1.2 Area & Circumference”

Items		Methods or Formula
Bulb	Outer Diameter	See “8.2.1.1 Distance (2D)”
	Inner Diameter	See “8.2.1.1 Distance (2D)”
	Outer Area	See “8.2.1.2 Area & Circumference”
	Inner Area	See “8.2.1.2 Area & Circumference”
Carotid Bifurcation	Outer Diameter	See “8.2.1.1 Distance (2D)”
	Inner Diameter	See “8.2.1.1 Distance (2D)”
	Outer Area	See “8.2.1.2 Area & Circumference”
	Inner Area	See “8.2.1.2 Area & Circumference”
ICA	Outer Diameter	See “8.2.1.1 Distance (2D)”
	Inner Diameter	See “8.2.1.1 Distance (2D)”
	Outer Area	See “8.2.1.2 Area & Circumference”
	Inner Area	See “8.2.1.2 Area & Circumference”
ECA	Outer Diameter	See “8.2.1.1 Distance (2D)”
	Inner Diameter	See “8.2.1.1 Distance (2D)”
	Outer Area	See “8.2.1.2 Area & Circumference”
	Inner Area	See “8.2.1.2 Area & Circumference”
Carotid Stenosis 1-4	Outer Diameter	See “8.2.1.1 Distance (2D)”
	Inner Diameter	See “8.2.1.1 Distance (2D)”
	Outer Area	See “8.2.1.2 Area & Circumference”
	Inner Area	See “8.2.1.2 Area & Circumference”
C.Iliac A	Outer Diameter	See “8.2.1.1 Distance (2D)”
	Inner Diameter	See “8.2.1.1 Distance (2D)”
	Outer Area	See “8.2.1.2 Area & Circumference”
	Inner Area	See “8.2.1.2 Area & Circumference”
Ex. Iliac A	Outer Diameter	See “8.2.1.1 Distance (2D)”
	Inner Diameter	See “8.2.1.1 Distance (2D)”
	Outer Area	See “8.2.1.2 Area & Circumference”
	Inner Area	See “8.2.1.2 Area & Circumference”
IIA	Outer Diameter	See “8.2.1.1 Distance (2D)”
	Inner Diameter	See “8.2.1.1 Distance (2D)”
	Outer Area	See “8.2.1.2 Area & Circumference”
	Inner Area	See “8.2.1.2 Area & Circumference”

Items		Methods or Formula
CFA	Outer Diameter	See “8.2.1.1 Distance (2D)”
	Inner Diameter	See “8.2.1.1 Distance (2D)”
	Outer Area	See “8.2.1.2 Area & Circumference”
	Inner Area	See “8.2.1.2 Area & Circumference”
DFA	Outer Diameter	See “8.2.1.1 Distance (2D)”
	Inner Diameter	See “8.2.1.1 Distance (2D)”
	Outer Area	See “8.2.1.2 Area & Circumference”
	Inner Area	See “8.2.1.2 Area & Circumference”
Int Jug V	Anterior-Posterior	See “8.2.1.1 Distance (2D)”
	Transverse	See “8.2.1.1 Distance (2D)”
	Checklist	/
C.Iliac V	Anterior-Posterior	See “8.2.1.1 Distance (2D)”
	Transverse	See “8.2.1.1 Distance (2D)”
	Checklist	/
Ex. Iliac A	Anterior-Posterior	See “8.2.1.1 Distance (2D)”
	Transverse	See “8.2.1.1 Distance (2D)”
	Checklist	/
IIV	Anterior-Posterior	See “8.2.1.1 Distance (2D)”
	Transverse	See “8.2.1.1 Distance (2D)”
	Checklist	/
CFV	Anterior-Posterior	See “8.2.1.1 Distance (2D)”
	Transverse	See “8.2.1.1 Distance (2D)”
	Checklist	/
DFV	Anterior-Posterior	See “8.2.1.1 Distance (2D)”
	Transverse	See “8.2.1.1 Distance (2D)”
	Checklist	/

8.3.5.2 Doppler Vascular Measurement

Table 35 Doppler Vascular Measurement

Items		Methods or Formula
Carotid	CCA	See “8.2.3.5 D Trace”
	ICA	See “8.2.3.5 D Trace”

Items		Methods or Formula
	ECA	See "8.2.3.5 D Trace"
	Bulb	See "8.2.3.5 D Trace"
	Carotid Bifurcation	See "8.2.3.5 D Trace"
Lower Extremity Artery	C.Iliac A	See "8.2.3.5 D Trace"
	Ex.Iliac A	See "8.2.3.5 D Trace"
	IIA	See "8.2.3.5 D Trace"
	CFA	See "8.2.3.5 D Trace"
	DFA	See "8.2.3.5 D Trace"
CCA (Sten)	Pre Sten	See "8.2.3.5 D Trace"
	Sten	See "8.2.3.5 D Trace"
	Post Sten	See "8.2.3.5 D Trace"
ICA (Sten)	Pre Sten	See "8.2.3.5 D Trace"
	Sten	See "8.2.3.5 D Trace"
	Post Sten	See "8.2.3.5 D Trace"
ECA (Sten)	Pre Sten	See "8.2.3.5 D Trace"
	Sten	See "8.2.3.5 D Trace"
	Post Sten	See "8.2.3.5 D Trace"
Bulb (Sten)	Pre Sten	See "8.2.3.5 D Trace"
	Sten	See "8.2.3.5 D Trace"
	Post Sten	See "8.2.3.5 D Trace"
Carotid Bifurcation (Sten)	Pre Sten	See "8.2.3.5 D Trace"
	Sten	See "8.2.3.5 D Trace"
	Post Sten	See "8.2.3.5 D Trace"
Carotid Stenosis 1-4	Pre Sten	See "8.2.3.5 D Trace"
	Sten	See "8.2.3.5 D Trace"
	Post Sten	See "8.2.3.5 D Trace"
C.Iliac (Sten)	Pre Sten	See "8.2.3.5 D Trace"
	Sten	See "8.2.3.5 D Trace"

Items		Methods or Formula
	Post Sten	See “8.2.3.5 D Trace”
Ex.Iliac (Sten)	Pre Sten	See “8.2.3.5 D Trace”
	Sten	See “8.2.3.5 D Trace”
	Post Sten	See “8.2.3.5 D Trace”
IIA (Sten)	Pre Sten	See “8.2.3.5 D Trace”
	Sten	See “8.2.3.5 D Trace”
	Post Sten	See “8.2.3.5 D Trace”
CFA (Sten)	Pre Sten	See “8.2.3.5 D Trace”
	Sten	See “8.2.3.5 D Trace”
	Post Sten	See “8.2.3.5 D Trace”
DFA (Sten)	Pre Sten	See “8.2.3.5 D Trace”
	Sten	See “8.2.3.5 D Trace”
	Post Sten	See “8.2.3.5 D Trace”
C.Iliac V	PV	See “8.2.3.5 D Trace”
	Reflux	/
	Checklist	/
Ex.Iliac V	PV	See “8.2.3.5 D Trace”
	Reflux	/
	Checklist	/
IIV	PV	See “8.2.3.5 D Trace”
	Reflux	/
	Checklist	/
CFV	PV	See “8.2.3.5 D Trace”
	Reflux	/
	Checklist	/
DFV	PV	See “8.2.3.5 D Trace”
	Reflux	/
	Checklist	/

8.3.5.3 Vascular Study and Calculation

➤ IMT

IMT (Intima-Media Thickness) refers to the vertical dimension between LI (Lumen-Intima) and MA (Media-Adventitia).

Perform the following steps:

1. In 2D mode, press the **[Caliper]** button on the control panel to start measurement.
2. Click **[IMT(NEAR)]** or **[IMT(FAR)]** in the measurement menu and the ROI box appears.
3. Move the cursor to the start point of ROI and then press the **[Set]** button. Roll the trackball to adjust the ROI area and then press the **[Set]** button. Two auto trace lines appear in the ROI box. Results are displayed in the result window.

NOTE:

- Please freeze the image before starting IMT measurement.
- Make sure that you select the right vessel wall (Near/ Far) before IMT measurement; otherwise wrong calculation may result.

➤ Stenosis D

Measure Normal Diam and Resid Diam, calculates Stenosis D.

$$\text{Stenosis } D = (D_1 - D_2) / D_1 \times 100\%$$

Where D_1 is Normal Diam and D_2 is Resid Diam.

➤ Stenosis A

Measure Normal Area and Resid Area, calculates Stenosis A.

$$\text{Stenosis } A = (A_1 - A_2) / A_1 \times 100\%$$

Where A_1 is Normal Area and A_2 is Resid Area.

➤ ICA/CCA(PS)

Measure the flow velocity ratio between ICA and CCA to calculate the stenosis.

Measure PS value of ICA and CCA distal by D trace method of Doppler general measurement, and the system automatically calculates the stenosis.

➤ ABI

Measure the Ankle Systolic Pressure (ASP) and Brachial Systolic Pressure (BSP) on Doppler image to calculate Ankle Brachial Index (ABI).

$$ABI = ASP / BSP$$

Chapter 9 Report

After the measurement is completed, the relevant measurement data will be displayed in the report.

9.1 View the Report

Press the **[Report]** on the control panel to enter the report screen of current animal.

The screenshot shows a software interface for generating a report. On the left, there is a sidebar with a 'Report Type' dropdown menu set to 'Vascular'. Below this are buttons for 'Save Comment', 'Load Comment', 'Print', 'Preview', and 'Setting'. At the bottom of the sidebar are 'Load Report' and 'Save Report' buttons. The main area contains a form with fields for 'Name', 'DOB', 'Gender', 'Operator', 'ID', 'Age', 'Ref. Physician', 'Host', 'Animal No.', 'Animals', 'BP(R)', 'BP(L)', 'Height', and 'Weight'. Below these fields is a 'Comment' text area. At the bottom of the main area are buttons for 'Previous', 'Next', 'Clear', 'Export', 'Save', and 'Cancel'.

Figure 42 Report

- NOTE:**
- The report shows the three latest values and a final value for the measurement.
 - The report only displays the measurement data displayed by default for the corresponding template.
 - General report only displays the caliper measurement data.

Table 36 Button Functions

Item	Description
Load Report	Click to preview, export or print a saved report
Save Report	Click to save the current report in PDF
Previous/ Next	Click [Previous] or [Next] to flip the pages if the report has more than one page
Export	Click to export report in PDF
Clear	Click to delete comments
Print	Click to print the current report
Preview	Click to preview the current report
Setting	Click to open the print Setting Dialog box
Save	Click to save comment as template

Item	Description
Comment	
Load Comment	Click to load saved comment
Add Image	Check the thumbnail in the Clipboard to add image
Save	Click to save current setting and return to the Home screen
Cancel	Click to cancel all modifications and return to the Home screen
⤴/⤵	Click to go to the previous/next page.
⏮/⏭	Click to go to the first/last page.
+	Click to open the image gallery.

9.2 Edit the Report

9.2.1 Comment

9.2.1.1 Add Comment

Perform the following steps:

1. Move the cursor over the comment box and press the **[Set]** button.

NOTE: The comment box is at the bottom of the report page. For reports with more than one page, please click **[Next]** to view the comments.

2. Enter comments in the comment box.

9.2.1.2 Load Comment

Click **[Load Comment]** to load saved comment.

9.2.1.3 Save Comment

Click **[Save Comment]** to save current comment as template.

9.2.2 Add Image

Images saved in the current exam can be added to the report.

Perform the following steps:

1. Click **[+]** to open the Image gallery. The column on the left displays the alternative ultrasonic images and the list on the right displays the selected ultrasonic images.
2. Add or remove Images.

Operation	Description
Add Image	1) Select the image you want to add from the left column. 2) Click [>] to add the selected image of the left column to the right column. Or Click [>>] to add all the selected images of the left column to the right column.
Remove Image	1) Select the image you want to add from the left column. 2) Click [<] to remove the selected images from the right column to the left column. Or Click [<<] to remove all the selected images from the right column to the left column.

9.3 Review the Report

Click [**Review Report**] to view the report.

NOTE: When reviewing, reports cannot be edited.

9.4 Print the Report

Click [**Print**] to print the report.

NOTE: Add the printer service prior to printing the report.

9.5 Back up the Report

NOTE: Save the report prior to loading or exporting the report.

9.5.1 Save

Click [**Save Report**] to save current report.

9.5.2 Load

Click [**Load Report**] to download existed report.

9.5.3 Export

1. Click [**Export**] to open the Export Wizard and set relevant parameters.
2. Click the [**Drive**] drop-down box to select the report export location.
3. Click the [**Type**] drop-down box to select the format of the exported report.
4. Select the directory where you want to export the report. You can also create or rename a new directory as needed.

Operation	Description
New	Create a new directory.
Rename	Rename the selected directory.

- Click **[OK]** to export the current report.

Chapter 10 Animal Data Management

After the animal image is acquired and processed, you can store and review the animal image or export the animal data to a USB storage device, drive (compatible format: CDFS) or DICOM server for future viewing.

10.1 Storage

Image and cine are saved to the system by default.

You can also back up data to a removable device or DICOM server. For details, see “10.5 Exporting Image/Data”.

10.1.1 Image Storage

In the freeze or real-time status, press the **[Save 1]** button on the control panel, the system will automatically save the current image to the current animal database. Saved images are displayed as thumbnails on the clipboard.

10.1.1.1 Image Saving Area

The system saves the standard area by default, and you can also set to save the image area. For details, refer to “4.2.3 Image”.

10.1.1.2 Image Saving Button

The **[Save 1]** button on the control panel is set to save a single frame image by default.

You can also define new button for image saving as needed. For details, refer to “4.2.5 Customize”.

10.1.2 Cine Storage

In the freeze or real-time status, press the **[Save2]** button on the control panel, the system will automatically save the cine to the current animal database.

10.1.2.1 Cine Length

For details, refer to “4.2.3 Image”.

10.1.2.2 Cine Saving Button

The **[Save 2]** button on the control panel is set to save cine by default. You can also define new button for cine saving as needed. For details, refer to “4.2.5 Customize”.

10.2 Image Viewing

Previous animal images/data can be viewed through the Station screen, and current animal images and data can also be viewed through other screens.

10.2.1 Current Animal

Image and cine of current animal can be viewed through the clipboard, review screen, and Station screen.

10.2.1.1 Through Clipboard

1. In the real-time or frozen status, press the **[Cursor]** button on the control panel to display cursor.
2. Locate the desire image / cine by clicking corresponding keys of the clipboard.
 - Click ▼ / ▲ to scroll up and down the pages of the thumbnail images.
 - Click ■ / ■■ to switch the display format between single window and dual window.
3. Roll the trackball, move the cursor to the desire thumbnail, double-click the **[Set]** button, and the screen displays the image in original size. To view cine, double-click the desire thumbnail to enter the cine replay status, the user can manually play the cine or play the cine automatically.
 - While viewing the image, replay, zooming, measurements are also available.
 - Press the **[Freeze]** button on the control panel to freeze the image and return to the home screen.

10.2.1.2 Though Station Screen

1. Press the **<Station>** key on the keyboard to enter the Station screen. The current animal is selected by default in the animal information list, and the clipboard displays the thumbnail image of the animal.

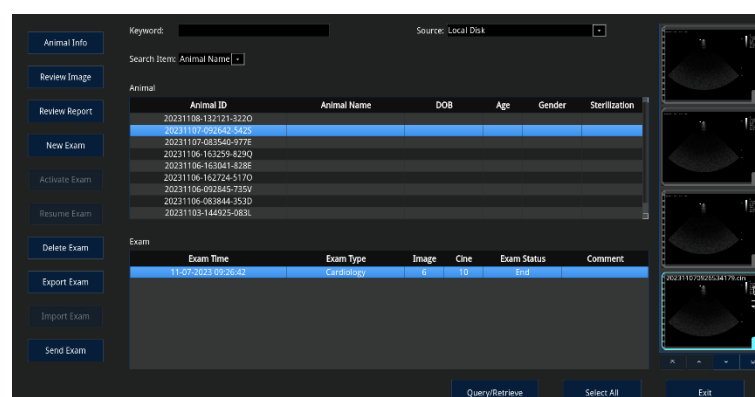


Figure 43 Station Screen

2. Move the cursor to the desire thumbnail image and double-click the **[Set]** button to enter the Home screen to view the image in original size.

10.2.1.3 Through Review Screen

1. Press the **<Station>** key on the keyboard to enter the Station screen. And then click **[Review Image]** to enter the Review screen of current animal.

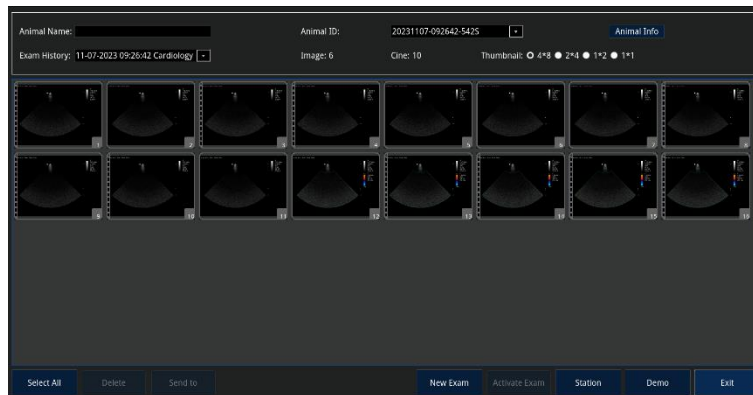


Figure 44 Review Screen

2. Roll the trackball, move the cursor to the desire thumbnail, double-click the **[Set]** button, and the screen displays the image in original size.

10.2.2 Previous Animals

To view data of previous animal through Station screen:

1. Press the **<Station>** key on the keyboard to enter the Station screen.
2. Search the desired animal.
 - Select the data source and search item, enter the keyword to search the desired animal.
 - Drop down the scroll bar on the right side of the animal information list to locate the desired animal.
3. Select the desired animal.
 - Move the cursor to the desire animal and double-click the **[Set]** button to enter the review screen to view the data of the animal.

10.2.2.1 Animal Information

Click **[Animal Info]** to enter the Animal screen to check basic information and exam information of desired animal.

10.2.2.2 Image

- The clipboard displays the thumbnail image of the animal. Click **^/~/X/⌵** to scroll through the thumbnail images, move the cursor to the desired image, and double-click the **[Set]** button to view the image.
- Or click **[Review Image]** to enter the Review screen, move the cursor to the desired image, and double-click the **[Set]** button to view the image.

10.2.2.3 Report

Click **[Review Report]** to view the report.

10.3 Delete Image/Data

10.3.1 Current Animal

10.3.1.1 Delete image through Clipboard

1. Select image.
 - Click  /  to scroll up and down the pages of the thumbnail images.
 - Click  /  to switch the display format between single window and dual window.
2. Move the cursor on the thumbnail of the image you want to delete and the delete icon “” displays.
3. Click “” icon to delete the image.

10.3.1.2 Delete image through Station screen

1. Press the **<Station>** key on the keyboard to enter the Station screen.
2. Move the cursor on the thumbnail of the image you want to delete and the delete icon “” displays.
 - Click  /  /  /  to scroll through the thumbnail images.
3. Click “” to delete the image.

10.3.1.3 Delete image through Review screen

Perform the following steps:

1. Press the **<Station>** key on the keyboard to enter the Station screen, and then click **[Review Image]** to enter the Review screen.
2. Move the cursor to select one or more thumbnail images.
 - Click “” to delete a specific image.
 - Click **[Select All]** to select all images.
3. Click **[Delete]** to delete the selected images.

10.3.2 Previous Animals

Perform the following steps:

1. Press the **<Station>** key on the keyboard to enter the Station screen.

2. Search desired animal.
 - Select the data source and search item, enter the keyword to search the desired animal.
3. Select desired animal.
 - Roll the trackball over the desired animal, press the **[Set]** button.
4. Delete animal data.
 - Delete image: move the cursor to the image to be deleted, click “” to delete the image; or click **[Review Image]** to enter the animal screen and delete image.
 - Delete animal data: click **[Delete Exam]**, and then click **[OK]** in the pop-up dialog box to delete the animal data.
 - Delete all animal data: **[Select All]** to select all animals. Click **[Delete Exam]** and then click **[OK]** in the pop-up dialog box to delete all animal data.

10.4 Image/Data Recovery

Deleted animal data will be cached in the recycle bin.

Due to the space limitations of the hard disk, the recycle bin can only cache animal data deleted within the past 30 days.

To recovery image/data, please perform the following steps:

1. Click the “” icon in the status bar to enter the recycle bin screen.
2. Select desired animal image or data.
 - Click **[Restore]** to restore the selected image/data.
 - Click **[Restore All]** to restore all images and data.
 - Click **[Delete]** to delete the selected image/data.
 - Click **[Delete All]** to delete all images and data.

10.5 Exporting Image/Data

The system supports exporting animal information, image and report to a USB storage device, drive (compatible format: CDFS) or DICOM server.

- NOTE:**
- The data in this system is exported in raw data format or DICOM format with different resolution, so the exported image is not the same as the image seen on the system display.
 - When connecting the external media, please check if the status bar displays the corresponding icon. If the icon is not displayed, re-connect the external media.
 - To ensure data security, please export important data regularly.

10.5.1 Exporting to USB Storage Device

10.5.1.1 Export Animal Data to USB Storage Device

Perform the following steps:

1. Connect the USB storage device to the system via the USB port and the status bar displays the “” icon.
2. Press the **<Station>** key on the keyboard to enter the Station screen.
3. Select the animal information you want to export.
 - Select the desired animal: search the animal information via the search items in the animal list.
 - Select all animals: click **[Select All]**.
4. Click **[Export Exam]** to open the Export Exam dialog box.
5. Set the export parameter.
 - 4) Click **[Destination]** drop-down box to select export destination.
 - 5) Check **[Original Format]** or **[DICOM Format]** to select the export format.
 - 6) Select the cine zoom mode, cine compression mode, and cine compression ratio.
 - 7) Set whether to delete local animal exam information after export.
 - Select **[Delete after exporting]**, and then click **[Delete Exam]** to delete animal data.
 - Select **[Delete after exporting]**, and then click **[Delete Image]** to delete animal image.
6. Click **[Export]** to export exam.

10.5.1.2 Remove the USB Storage Device

Move the cursor over the “” icon, press the **[Set]** button, select the USB storage device to be removed in the pop-up dialog box and click **[OK]** to remove the USB device safely.

10.5.2 Exporting to DVD Disc (Optional)

Perform the following steps:

1. Insert a disc into the DVD drive and the status bar displays the “” icon.
2. Press the **<Station>** key on the keyboard to enter the Station screen.
3. Select the animal information you want to export.
 - Select the desired animal: search the animal information via the search items in the animal list.
 - Select all animals: click **[Select All]**.
4. Click **[Export Exam]** to open the Export Exam dialog box.

5. Set the export parameter. (Setting method is the same as exporting to USB storage device. See “10.5.1.1 Export Animal Data to USB Storage Device” for details.
6. Click **[Export]** to export exam.
7. The recording process bar displays and the disc ejects automatically when recording is complete.
8. Remove the disc.

10.5.3 Exporting to DICOM Server

The DICOM Server is purchasable. Please confirm the function is purchased and installed before use.

Export animal images to the DICOM server, refer to “11.2.1 DICOM Storage” for details.

10.6 Disk Space Detection

Display disk space information such as disk capacity, available capacity, and disk usage (occupancy rate).

Place the cursor over the disk icon “” in the status bar to view the disk space information.

10.7 Task Manager

The user can enter the task manager screen to view the status of exam sending, importing, and exporting.

NOTE: The information displayed in Task Manager Screen will be cleared after restarting.

Click the task manager icon “” in the status bar to enter the task manager screen.

10.8 Image Demo

Image demo function is used for demonstration of the images stored. Selected image files are played according to the customized order.

To perform image demonstration:

1. Press the **<Station>** key on the keyboard to enter the Station screen, and then click **[Review Image]** to enter the Review screen. Click **[Demo]** to enter the Demo Screen. Edit the content to be played and make related settings as needed.

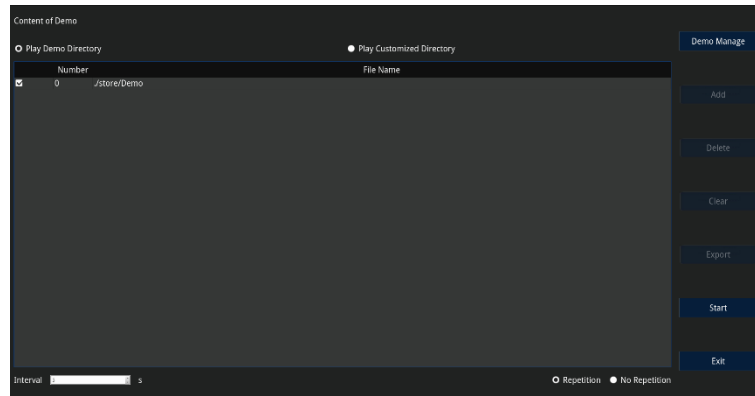


Figure 45 Demo

Table 37 Demo

Item		Description
Content of Demo	Play Demo Directory	Demo directory is the folder in hard disk, where the factory DEMO is stored. The system plays the images in this folder when performing demonstration. This directory is managed via [Demo Manage] .
	Play Customized Directory	Customized directory stores displayed files. You can add/delete demo images. The system plays the selected images in this folder when performing demonstration.
Demo Manage		Click to enter demo catalog management. Click [>] to add image to demo catalog; Click [<] to delete the selected image in demo catalog; Click [<<] to delete all images in demo catalog.
Add file		To add file to the customize catalog.
Delete		Delete file in the customize catalog.
Clear (Reserved function)		Clear all files in the customize catalog.
Export (Reserved function)		Export the selected file to the external storage devices.
Start		Start image demonstration.
Exit		Exit image demonstration.
Interval		Set the demo interval between images.
Repetition / No Repetition		Set whether to repeat the demonstration or exit after a demonstration is completed.

2. Select catalog to be demonstrated, and click **[Start]** to begin the demonstration.
3. Click **[Exit]** to exit image demo function.

Chapter 11 DICOM

Digital Imaging and Communications in Medicine (DICOM) Standard is an international normative protocol for communication of medical digital images. DICOM service enables you to:

- Search for animal information archived on the DICOM server (working list) and import the animal information to the device for reviewing.
- Send animal information and images on the system to the DICOM storage server.
- Send the image saved on the system to the DICOM print server for image printing.

NOTE: The DICOM Server is purchasable. Please confirm the function is purchased and installed before use.

11.1 DICOM Preset

11.1.1 DICOM Local Preset

Preset the network properties for DICOM server connection.

Enter the DICOM local preset screen via **[Preset]** (press **<Setup>**) → **[Network Preset]** → **[DICOM Local]**.

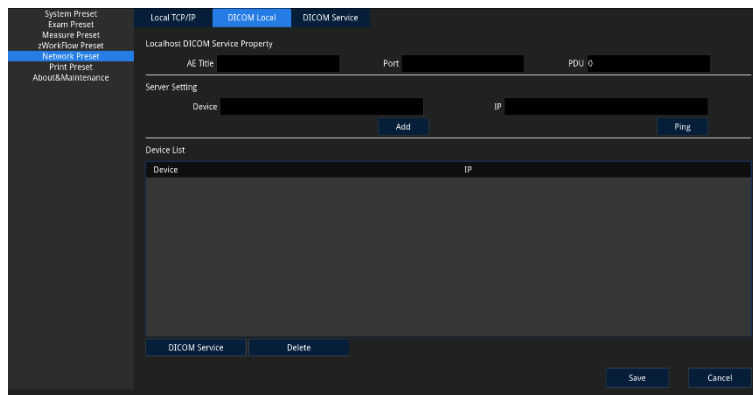


Figure 46 DICOM Local

Table 38 DICOM Local

Item	Description
AE Title	Application Entity (AE) title which is used for device identification. The AE title should be consistent with that of the acceptable SCU preset in the server.
Port	Always the same as the server port.
PDU	The maximum PDU data package size.
Device	Name of the device supporting DICOM services.

Item	Description
IP	IP address of the DICOM server.
Add	Add the server to the server list.
Ping	Check network connectivity between the system and DICOM server.
Device List	Display the added devices.
DICOM Service	Set the DICOM servers. For details, refer to “11.1.2 Service Preset”.
Delete	Remove the selected server from the device list.

To connect a DICOM server, perform the following steps:

1. Use a network cable to connect the device to the LAN of DICOM server.
2. Set the local network. (Refer to “4.6 Network Preset” for details)
3. Set DICOM server properties.
 - Enter the AE title, port, PDU, device name and IP address.
4. Click **[Add]** to add the server to the device list.
5. Click **[Ping]** to check the connection, the prompt information is displayed in the status bar at the bottom of the screen.
6. Click **[Save]** to save current setting and return to the Home screen.

NOTE: The AE Title should be consistent with the SCU AE Title preset in the server (PACS/RIS/HIS), for example, if the AE Title preset of the printer server is “Printer”, and the SCU AE Title is “Machine”, then the AE Title of local should be “Machine” in the figure above, while the AE Title of the printer server should be “Printer”.

11.1.2 Service Preset

The service preset is mainly used to add or delete DICOM services in a DICOM server, set the service name, port address, and so on.

DICOM service consists of Storage, Print, Worklist, MPPS, Storage Commitment, and Query/Retrieve.

11.1.2.1 Storage

Storage server connection properties and image storage format settings can be found in the Storage Service Preset screen.

Enter the Storage Service Preset screen via **[Preset]** (press **<Setup>**) → **[Network Preset]** → **[DICOM Service]** → **[Storage]**.

Figure 47 DICOM Service-Storage

Table 39 DICOM Service-Storage

Item	Description
Device	Click the drop-down box to select an added device.
Service Name	Enter a service name. Default is storage-default.
AE Title	Enter the AE title. The AE Title here should be consistent with that of the storage server.
Port	Enter the port number for the storage server.
Maximum Retries	Set the maximum retries.
Interval Time (Sec)	Set the interval time for connection retry.
Timeout (Sec)	Refers to the amount of time after which the system will stop trying to establish a connection to the service.
Cine Zoom Mode	Select the cine zoom mode.
Compression Mode	Select the compression mode.
Compression Ratio	Select the compression ratio.
Color Mode	Select the color mode.
Allow Multiframe	Select if support multi-frame saving.
Max Frame Rate	Set the frame range of transferring cine file into DCM multi-frame file.
3D/4D	Set the 3D/4D image transfer mode.
Storage Options	Enable or disable structured reporting sending.
Encapsulated PDF	Select whether to encapsulate PDF reports in DICOM standard format.
Add	Add a server to the server list.

Item	Description
Cancel	Cancel parameter preset.
Update	Select a server in the service list, change the parameters and click [Update] to update the parameters of the server.
Service List	Display the connected storage server list.
Delete	Remove the selected server from the device list
Default	Select an item in the server list as the default server, and the default server is marked with a “Y”.
Verify	Verify the network connectivity between the system and storage server.

➤ **Preset Storage Server**

To preset a storage server, please perform the following steps:

1. Click **[Device]** drop-down box to select an added device.
2. Enter the AE title and port consistent with the DICOM storage server, and enter other properties.
3. Select certain service in the service list; click **[Verify]** to verify the network connectivity.
4. Click **[Save]**, the system saves the settings and returns to the Home screen.

NOTE: Not all SCP support verification. Please confirm whether the SCP supports the verification before verification.

➤ **Change Server Parameters**

1. Double click the server you want to change parameter to display parameter dialog.
2. Change the parameters as needed, and click **[Update]** to update and save the current parameters.

➤ **Set Default Server**

Select a server in the service list, click **[Default]** and the default server is marked with a “Y”.

11.1.2.2 Print

Service and print attributes, and print server connection can be found in print service screen. Print server setting is similar to storage server setting, refer to “11.1.2.1 Storage” for details.

Enter the print service preset screen via **[Preset]** (press **<Setup>**) → **[Network Preset]** → **[DICOM Service]** → **[Print]**.

Figure 48 DICOM Service-Print

Table 40 DICOM Service-Print

Item	Description
Device	Click the drop-down box to select an added device.
Service Name	Enter a service name. Default is print-default.
AE Title	Enter the AE title. The AE Title here should be consistent with that of the print server.
Port	Enter the port number for the print server.
Maximum Retries	Set the maximum retries.
Interval Time (Sec)	Set the interval time for connection retry.
Timeout (Sec)	Refers to the amount of time after which the system will stop trying to establish a connection to the service.
Copies	Copies of each page.
Settings	Set the printer type of the printer
Film Orientation	Set the film orientation.
Priority	Set the priority of color printing.
Film Size	Set the film size.
Display Format	Specify the quantity of images per page to print. E.g. STANDARD\2, 3 means 6 images are printed for each page.
Medium Type	Set the medium type of the printer.
Trim	Set whether to print the trim box around each image of the film.
Min Density	Enter the minimum density of the film.

Item	Description
Max Density	Enter the maximum density of the film.
Configuration Info	Enter configuration information.
Destination	Set where the file is exposed.
Magnification Type	Set the magnification type for image printing.
Add	Add a server to the server list.
Cancel	Cancel parameter preset.
Update	Select a server in the service list, change the parameters and click [Update] to update the parameters of the server.
Service List	Display the connected print server list.
Delete	Remove the selected server from the device list
Default	Select an item in the server list as the default server, and the default server is marked with a “Y”.
Verify	Verify the network connectivity between the system and print server.

Set the print attribute related parameters based on the actual printer requirements, for example:

- If the printer does not support **[Film Size]** as 8N*10N, do not set this size to the printer film size.
- As to **[Medium Type]**, Blue Film or Clear Film is usually used for black and white printing, and Paper is usually used for color printing. For details, please refer to the printer conformance statement.
- Other parameters can be reminded as default. If the printer has special requirements, please change the parameters according to the requirements of the printer.

11.1.2.3 Worklist

Worklist server connection properties and relevant settings can be found in the Worklist service preset screen. Worklist server setting is similar to storage server setting, refer to “11.1.2.1 Storage” for details.

Enter the Worklist service preset screen via **[Preset]** (press **<Setup>**) → **[Network Preset]** → **[DICOM Service]** → **[Worklist]**.

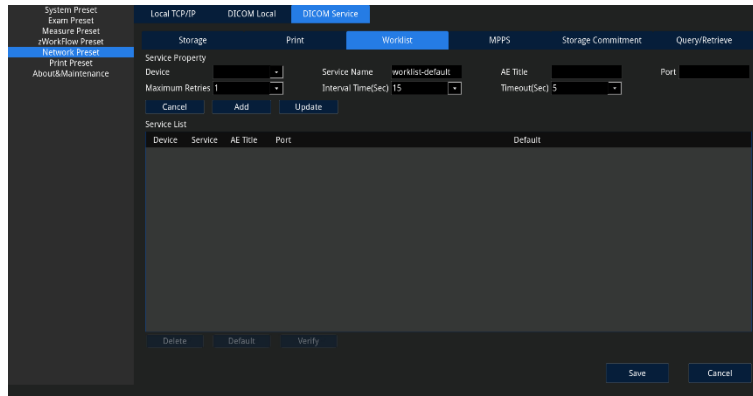


Figure 49 DICOM Service-Worklist

Table 41 DICOM Service-Worklist

Item	Description
Device	Click the drop-down box to select an added device.
Service Names	Enter a service name. Default is worklist-default.
AE Title	Enter the AE title. The AE Title here should be consistent with that of the worklist server.
Port	Enter the port number for the worklist server.
Maximum Retries	Set the maximum retries.
Interval Time (Sec)	Set the interval time for connection retry.
Timeout (Sec)	Refers to the amount of time after which the system will stop trying to establish a connection to the service.
Add	Add a server to the server list.
Cancel	Cancel parameter preset.
Update	Select a server in the service list, change the parameters and click [Update] to update the parameters of the server.
Services List	Display the connected worklist server list.
Delete	Remove the selected server from the device list
Default	Select an item in the server list as the default server, and the default server is marked with a “Y”.
Verify	Verify the network connectivity between the system and the worklist server.

11.1.2.4 MPPS

MPPS server connection properties and relevant settings can be found in the MPPS service preset screen. MPPS server setting is similar to storage server setting, refer to “11.1.2.1 Storage” for details.

Enter the MPPS service preset screen via **[Preset]** (press **<Setup>**) → **[Network Preset]** → **[DICOM Service]** → **[MPPS]**.

NOTE: When using MPPS, you need to set the MPPS server as the default server.

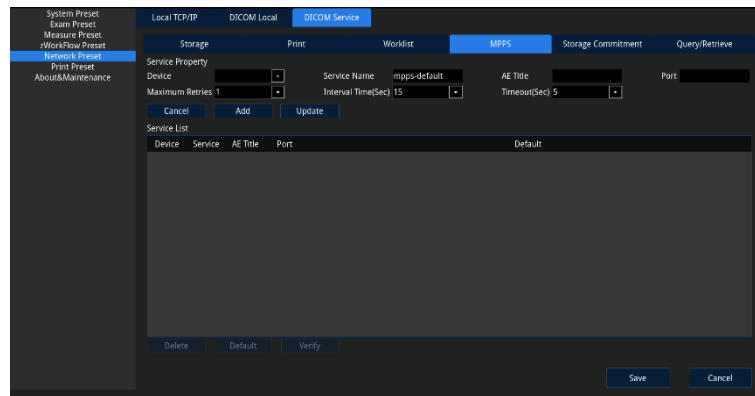


Figure 50 DICOM Service-MPPS

Table 42 DICOM Service-MPPS

Item	Description
Device	Click the drop-down box to select an added device.
Service Name	Enter a service name. Default is mpps-default.
AE Title	Enter the AE title. The AE Title here should be consistent with that of the mpps server.
Port	Enter the port number for the print server.
Maximum Retries	Set the maximum retries.
Interval Time (Sec)	Set the interval time for connection retry.
Timeout (Sec)	Refers to the amount of time after which the system will stop trying to establish a connection to the service.
Add	Add a server to the server list.
Cancel	Cancel parameter preset.
Update	Select a server in the service list, change the parameters and click [Update] to update the parameters of the server.
Service List	Display the connected mpps server list.

Item	Description
Delete	Remove the selected server from the device list
Default	Select an item in the server list as the default server, and the default server is marked with a “Y”.
Verify	Verify the network connectivity between the system and the mpps server.

11.1.2.5 Storage Commitment Preset

Storage Commitment server connection properties and relevant settings can be found in the storage commitment service preset screen. Storage commitment server setting is similar to storage server setting, refer to “11.1.2.1 Storage” for details.

Enter the MPPS service preset screen via **[Preset]** (press **<Setup>**) → **[Network Preset]** → **[DICOM Service]** → **[Storage Commitment]**.

Figure 51 DICOM Service-Storage Commitment

Table 43 DICOM Service-Storage Commitment

Item	Description
Device	Click the drop-down box to select an added device.
Service Name	Enter the service name. Default is sc-default.
AE Title	Enter the AE title. The AE Title here should be consistent with that of the Storage Commitment server.
Port	Enter the port number for the Storage Commitment server.
Maximum Retries	Set the maximum retries.
Interval Time (Sec)	Set the interval time for connection retry.
Timeout (Sec)	Refers to the amount of time after which the system will stop trying to establish a connection to the service.

Item	Description
Associated Storage Service	The associated storage server should be preset before storage commitment, only after the exam is sent out, can storage commitment be created.
Cancel	Cancel parameter preset.
Add	Add a server to the server list.
Update	Select a server in the service list, change the parameters and click [Update] to update the parameters of the server.
Service list	Display the connected storage commitment server list.
Delete	Remove the selected server from the device list
Default	Select an item in the server list as the default server, and the default server is marked with a “Y”.
Verify	Verify the network connectivity between the system and the storage commitment server.

11.1.2.6 Query / Retrieve Preset

Query/Retrieve server connection properties and relevant settings can be found in the Query/Retrieve service preset screen. Query/Retrieve server setting is similar to storage server setting, refer to “11.1.2.1 Storage” for details.

Enter the Query/Retrieve service preset screen via **[Preset]** (press **<Setup>**) → **[Network Preset]** → **[DICOM Service]** → **[Query/Retrieve]**.

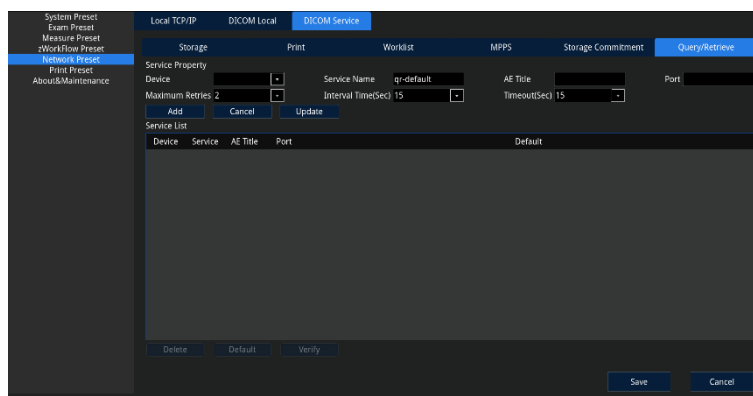


Figure 52 DICOM Service-Query/Retrieve

Table 44 DICOM Service-Query/Retrieve

Item	Description
Device	Click the drop-down box to select an added device.

Item	Description
Service Name	Enter a service name. Default is qr-default.
AE Title	Enter the AE title. The AE Title here should be consistent with that of the query/retrieve server.
Port	Enter the port number for the query/retrieve server.
Maximum Retries	Set the maximum retries.
Interval Time (Sec)	Set the interval time for connection retry.
Timeout (Sec)	Refers to the amount of time after which the system will stop trying to establish a connection to the service.
Add	Add a server to the server list.
Cancel	Cancel parameter preset.
Update	Select a server in the service list, change the parameters and click [Update] to update the parameters of the server.
Service List	Display the connected query/retrieve server list.
Delete	Remove the selected server from the device list
Default	Select an item in the server list as the default server, and the default server is marked with a “Y”.
Verify	Verify the network connectivity between the system and the query/retrieve server.

11.2 DICOM Service

After completed all DICOM presets, you are ready for DICOM image storage, DICOM image printing, work list, MPPS, storage delegation and query/acquisition services.

NOTE: Before using DICOM services, please perform verification to ensure that the system is properly connected to the DICOM server.

11.2.1 DICOM Storage

DICOM storage service sends animal image or data to storage server for remote storage.

Perform the following steps:

1. Save images. Refer to “10.1 Storage” for details.
2. Send images/data to the DICOM storage server via following screens:

- Move the cursor over the thumbnail of the image you want to send in the Home screen, click “” icon on the image.
 - Press **<Station>** key on the keyboard and click **[Review Image]** to enter the Review screen. Move the cursor over the thumbnail of the image you want to send, click “” icon on the image or click **[Send]** to send the selected images.
 - Press the **<Station>** key on the keyboard to enter the Station screen. Select desired animal and click **[Send Exam]** or move the cursor over the thumbnail of the image you want to send, click “” icon on the image.
3. A sending dialog box pops up. Select DICOM and storage server as needed.
 4. Click **[OK]** to send the image/data to the storage server.

11.2.2 DICOM Print

DICOM Print service sends animal image to print server for remote printing. Preset the print server before using DICOM Print service.

Perform the following steps:

1. Save images. Refer to “10.1 Storage” for details.
2. Send image to DICOM Print Server via following screens:
 - Move the cursor over the thumbnail of the image you want to send in the Home screen, click “” icon on the image.
 - Press **<Station>** key on the keyboard and click **[Review Image]** to enter the Review screen. Move the cursor over the thumbnail of the image you want to send, click “” icon on the image or click **[Send]** to send the selected images.
 - Press the **<Station>** key on the keyboard to enter the Station screen. Select desired animal and click **[Send Exam]** or move the cursor over the thumbnail of the image you want to send, click “” icon on the image.
3. A sending dialog box pops up. Select DICOM and print server as needed.
4. Click **[OK]** to send the image/data to the print server.

11.2.3 DICOM Worklist

The DICOM Worklist Service is used to query or retrieve animal information stored in the server, which can be imported into the system for viewing and performing new exam. Preset the DICOM Worklist server before using DICOM Worklist service.

To retrieve Animal information (DICOM), perform the following steps:

1. Press the **[Patient]** button on the control panel to enter the animal information screen. Click **[Worklist]** to display Worklist screen.

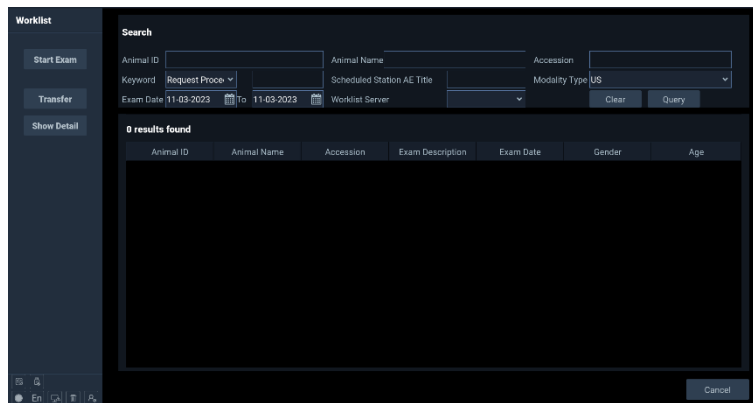


Figure 53 Worklist Screen

2. Query animal information:
 - 1) Set search condition among animal ID, animal name, accession number, keyword, scheduled station AE Title, device type, exam date, worklist server and other information to search for animals.
 - 2) Click **[Query]** to display animal information which meets the search conditions in the lower part of the screen. Or click **[Clear]** to clear the entered query criteria and the query results.
3. Select desired animal record in the displayed animal list:
 - **[Start Exam]**: click to return to the Home screen and start a new exam for the selected animal.
 - **[Transfer]**: click to import the selected animal information into the **[Animal Information]** screen for editing. After editing, click **[Save]** to start a new exam. Or click **[Cancel]** to return Home Screen without a new exam.
 - **[Show Detail]**: click to view the detailed animal information.
 - **[Cancel]**: click to exit worklist screen and return to the animal information screen.

11.2.4 DICOM MPPS

MPPS is used to send animal exam status to the MPPS server. This will facilitate the other systems to obtain the exam progress in time. Preset the DICOM MPPS server before using DICOM MPPS service.

When MPPS preset is done, the animal exam status will be sent to the MPPS server as follows:

- When start a new exam, the system sends an “N-CREATE” message to the MPPS server.
- After the image acquisition completes, the system sends an “N-SET COMPLETED” message to the MPPS server.
- When the image acquisition is abnormally terminated, the system sends “N-SET DISCONTINUED” to the MPPS server.

11.2.5 DICOM Storage Commitment

After the animal exam information or the structured report on the system is sent to the storage server, the system can detect whether the information transmission is successful through the storage commitment server. Preset the DICOM Storage Commitment server before using DICOM Storage Commitment service.

11.2.5.1 Send animal exam to DICOM storage server

Perform the following steps:

1. After completing the exam, press the **[EndExam]** button on the control panel to end the current exam.
2. Press the **<Station>** key on the keyboard to enter the Station screen.
3. Select the desired animal in the animal list, click **[Send Exam]**.
4. A sending dialog box pops up. Select DICOM and storage server as needed.
5. Click **[OK]**, the image and data will be sent to the DICOM storage server, and the storage commitment server will prompt the sending status in the prompt bar.

11.2.5.2 Auto send animal exam to DICOM storage server

Send images automatically to the DICOM storage server and perform storage commitment when the exam is done.

Set the auto function via **[Preset]** (press **<Setup>**) → **[System Preset]** → **[General]** → **[Send after Exam]**.

When the exam completes, the system prompts whether the exam information was successfully sent to the DICOM storage server.

11.2.6 DICOM Query / Retrieve

The query/retrieve server is used to query and retrieve the animal exam information from the designated server, so as to remotely obtain other exam information of the animal.

Preset the query/retrieve server before using DICOM query/retrieve service.

To query / retrieve animal information, please perform the following steps:

1. Press the **<Station>** key on the keyboard to enter the Station screen.
2. Click **[Query/Retrieve]** to enter query/retrieve screen.
3. Select the source server (query location) for accessing animal information, and the target server (retrieve location) in **[Server & Service]**.
4. Enter query information, such as an animal ID, animal name, serial number, keyword, or the time period to screen the animal.
 - Click **[Clear]** to clear the entered query conditions and results.
5. Click **[Query]** and the qualified animals are displayed in the animal list.

- If the list is more than one page, roll the right slider bar of the list to find the animal information.
 - Move the trackball and press the **<Ctrl> + [Set]** button to select more than one animals.
 - Click **[Select All]** to select all animals.
 - Click **[Cancel All]** to cancel multiple or all animals selected in the list.
6. Click **[Retrieve]**, the system will retrieve the selected animal record to the target server or local and the animal information displays in the animal list after completion.
 7. After completing retrieval, click **[Exit]** to see the retrieved animal records in the Station screen.

11.3 Structured Report

The system provides a common structured report that supports DICOM storage, DICOM storage commitment, and export to external storage devices in DCM format.

11.3.1.1 Send Structured Report to DICOM via Station screen

NOTE: Structured reports cannot be sent separately and can only be sent with DICOM images.

Perform the following steps:

1. Set up structured reports to be sent to the DICOM storage server along with the images.
 - Setting path: **[Preset]** (press **<Setup>**) → **[Network Preset]** → **[DICOM Service]** → **[Storage]** → **[Storage Option]** → **[Send DICOM SR]**.
2. After completing the exam, press the **[EndExam]** button on the control panel to end the current exam.
3. Press the **<Station>** key on the keyboard to enter the Station screen.
4. Click **[Send Exam]** to pop up the sending exam dialog box.
5. Select **[DICOM]** and storage server, and then click **[OK]** to confirm.

11.3.1.2 Export Structured Report to External Storage

Structured reports cannot be exported separately and can only be exported with animal data. When exporting animal data, if there is a structured report, the structured report will be exported to the external storage device as well.

Perform the following steps:

1. After completing the exam, press the **[EndExam]** button on the control panel to end the current exam.
2. Press the **<Station>** key on the keyboard to enter the Station screen.
3. Click **[Send Exam]** to pop up the sending exam dialog box.

4. Select **[Disk]**, check **[Export Report]** as needed and click **[OK]** to start exporting.

Chapter 12 Probe and Biopsy

Prior to the exam, the user must fully understand the function of the probe.

To ensure the performance and safety of the probe, regular cleaning, disinfection, and maintenance shall be taken.

12.1 Probe

This section mainly introduces the general operation of the probe.

12.1.1 Structure of Probe

The ultrasonic probes suitable for this system are all electronic scanning probes, which generates high-resolution images by transmitting ultrasonic waves into the human body and receiving echoes.

The basic structure of the probe is shown in the figure below. The orientation mark on the probe is consistent with the direction indicated by the probe mark “●” on the ultrasonic image.

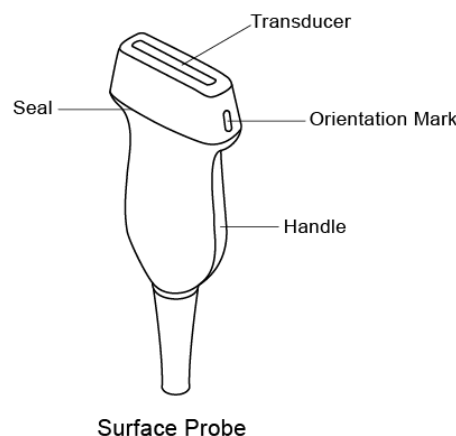


Figure 54 Structure of Probe

12.1.2 Probe Usage



- **DO NOT** use any probe not provided by the manufacturer, otherwise the console and probe will be damaged. In serious cases, fire and other accidents may result.
- Use the probe with care. Stop use immediately if the probe appears to be malfunctioning. Otherwise, electric shock and burns may result.
- Carefully inspect the probe sheath for damage or breakage before use. Do not use a damaged probe sheath to prevent infection.
- **DO NOT** use mineral oils, oily coupling gel, gels with any type of detergent or softener, and other unapproved materials to replace coupling gel supplied or recommended by the manufacturer.

Otherwise, probe damage may result.

- **Use qualified ultrasonic coupling gel and read the coupling gel manual carefully before use.**

Perform the following steps:

1. Check the probe. The probe may have potential damage during use and cleaning. Therefore, the following checks should be performed on the probe before use to ensure:
 - No cracks on the probe
 - No cracks on the front part of the probe
 - No scratch on the transducer surface
 - No expansion on the transducer surface
 - No cracks or any other damage on the cable sheath
 - No cracks or any other damage on the connector
 - No bent or broken pins
 - No cable damage
2. Connect the probe to the system. Refer to “3.6.1 Connect the Probe” for details.
3. Recognize the direction of probe and perform the exam.
4. After completing each exam, clean and disinfect the probe as required. Remove the probe sheath and dispose of the sheath in accordance with the medical specifications for bio-hazardous waste.

12.1.3 Probe Cleaning

After completing each exam, the probe and reusable parts should be thoroughly cleaned as required. Fail to do so may result in the probe and the bracket becoming sources of infection.



Warning

- **Never immerse the probe connector into liquid such as water or disinfectant. Immersion may cause electrical shock or malfunction.**
- **Prior to cleaning the probe, disconnect the probe from the ultrasonic system to avoid electric shock.**
- **When clean the probe, avoid impacting the probe with sharp or hard objects.**
- **Always wear sterile gloves to prevent infection when performing cleaning of probe.**
- **No cleaning and disinfecting may result in the probe becoming a source of infection.**

NOTE:

- **After the examination, wipe off the coupling agent thoroughly. Otherwise, the coupling agent may solidify and degrade the image quality of the transducer.**
- **DO NOT make the probe overheated (more than 55°C) during cleaning procedure. High temperature may result in probe deformation or damage.**

After each exam, the probe should be cleaned as required:

1. Disconnect the probe from the system.
2. Wear sterile gloves to prevent infection.
3. Rinse the probe with pure water for 2 minutes to remove foreign matters on the surface of the transducer. Or wipe the transducer with a soft lint-free cloth dipped in neutral enzyme detergent for 1 minute to further remove contaminants. Avoid using a brush, as it may damage the transducer.
4. After rinsing, wipe the surface of the transducer with a sterile cloth or gauze dipped in pure water for 1 minute to remove the residual detergent on the surface.
5. Dry the transducer using a sterile cloth. Do not dry the transducer by heating.

12.1.4 Probe Disinfection

After each exam, the probe and reusable parts should be thoroughly disinfected as required. Fail to do so may result in the probe and the bracket becoming sources of infection.



- **It is recommended to use the disinfectant listed in this manual and ensure that its concentration and probe immersion time meet the recommended requirements. Fail to do so may damage the probe and void the probe warranty; if the user has special purpose and requirements, ensure that the formulated solution concentration and probe immersion time are appropriate for the intended clinical use.**
- **The probe must be disinfected with a liquid chemical disinfectant that complies with local regulations.**
- **DO NOT use high pressure steam or ethylene oxide to contact with the probe.**
- **DO NOT the probe by heating under any circumstances. If the temperature exceeds 55°C, the probe will be damaged**
- **DO NOT allow any disinfectant to air dry on the probe.**
- **Before disinfecting the probe, please pay attention to the expiration date of the disinfectant and never use expired disinfectant.**
- **Always wear sterile gloves and to prevent infection.**

NOTE: Repeated disinfection will eventually damage the probe, please check the probe performance periodically.

12.1.4.1 Immersion Disinfection Limit

Never immerse the probe deeper than the line shows below for disinfection (the immersion limit also applies during normal use and performance evaluation).

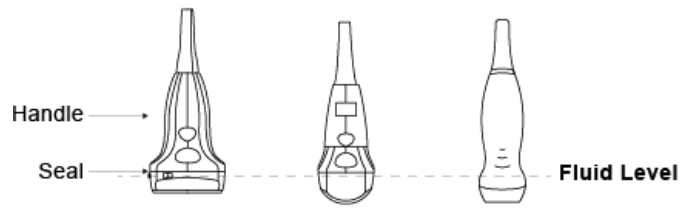


Figure 55 Immersion limitation for Different Probe Type

12.1.4.2 Disinfection for Surface Probe

After each exam, the surface probe should be disinfected as required.

Perform the following steps:

1. Wear sterile gloves to prevent infection.
2. Cleaning the probe. (Refer to “12.1.3 Probe Cleaning” for details)
3. Disinfect the probe according to the low-level disinfection method recommended in the table below.

Table 45 Low-level Disinfection

Disinfectant	Manufacturer	Active ingredient	Concentration	Manner of contact	Contact time
Cidex	J&J	OPA	0.55%	Soak	3 min

4. Rinse the transducer with plenty of sterile water for at least 1 minute to remove all chemical residues. Or follow the rinsing method recommended by the disinfectant manufacturer to rinse the transducer.
5. After rinsing, wipe the surface of the transducer with a sterile cloth dipped in sterile water for 1 minute to further remove any residual disinfectant on the surface.
6. Wipe off water on the transducer using a sterile cloth. Do not dry the transducer by heating.

NOTE:

- The recommended disinfectants listed in this manual are recommended because they are chemically compatible with the materials of the products, not because of their biological effects. For the biological effects of disinfectants, please refer to the guidance and recommendations provided by the disinfectant manufacturer, the US Food and Drug Administration, and the US Centers for Disease Control.
- If the disinfectant recommended in this manual is not selected, prepare the solution according to the disinfectant manufacturer’s instructions.

12.1.5 Probe Maintenance

The probe should be used, stored or transported under the conditions of “Appendix A Technical Specifications”.

12.1.5.1 Probe Transportation

To properly store the probe for transportation, please perform the following steps:

1. Before place the probe in the shipping container, make sure the probe is cleaned and sanitized to avoid contaminating the liner foam of the shipping container.
2. Carefully place the probe in the probe box.
3. Ensure the probe is totally in the box before covering the probe box.
4. Wrap the probe box in a plastic material with air bag (such as foam) and place the wrapped probe box into the cardboard box.

12.1.5.2 Probe Storage

To protect the probe, follow the guidelines below:

- Place the probe in the probe holder when the probe is temporarily idle.
- If the probe is not used for a long time, clean and disinfect the probe to ensure that the probe is completely dry before storing in the probe box.
- Prior to placing the probe, make sure the probe holder is clean and dry.
- Separately store the probe from other medical devices.

12.2 Biopsy



- **Physicians who use this system for biopsy must undergo professional ultrasound guidance training and strictly observe the operation requirements of biopsy to avoid unnecessary harm to animals.**
- **Before a biopsy procedure is performed, confirm that the needle-guided bracket is in good condition, and the biopsy guide line and the bracket must be calibrated.**
- **The biopsy guide line displayed on the ultrasound image is for reference only. During biopsy procedure, the operator should always monitor the position of the needle and confirm the correct needle position.**
- **DO NOT freeze the image during the biopsy procedure to avoid positioning errors.**
- **The operator should maintain a high concentration of attention during the biopsy procedure to avoid medical accidents.**
- **Gloves should be worn when performing biopsy procedure.**
- **Never allow to reuse the biopsy needle.**
- **A probe with sheath must be used during the biopsy procedure.**

12.2.1 Calibrate the Biopsy Guide Line

Calibrating the guide line is necessary before each biopsy procedure or changing biopsy angle.

Perform the following steps:

1. Install the needle-guided bracket.
2. Place the head of the probe in a liquid tank with distilled water.
3. Insert the puncture needle along the needle-guided bracket until the tip of the puncture needle is at the maximum depth of the water.
4. In B mode, press the **<Biopsy>** key to enter the Biopsy screen.

Item	Description
Biopsy Kit	Select bracket kit and angle.
Calibrate	Click to enter the biopsy calibration screen.
Double Line	Click to enable / disable double guide line function.
Line Type	Select the biopsy guide line type.
Biopsy Enhance	Click to enable / disable the biopsy enhance function.
Exit	Exit the biopsy screen.

5. Tap **[Biopsy Kit]** on the touch screen to select appropriate kit and angle.
6. Tap **[Calibrate]** on the touch screen to enter the biopsy guide line calibration screen.
7. Verify that the needle displayed on the ultrasound image matches the guide line. If not, adjust the guide line angle and position.
 - Rotate the knob under **[Position]** to adjust the guide line position.
 - Rotate the knob under **[Angle]** to adjust the guide line angle.
8. After calibration, click **[Save]** to save the adjustment.
 - To restore the factory settings, tap **[Restore]** on the touch screen and click **[Save]**.
9. Tap **[Exit]** on the touch screen to return to B mode, and then press **<Biopsy>** on the keyboard to exit the Biopsy screen.

12.2.2 Biopsy Procedure

Before performing a biopsy procedure, determine the size of the biopsy target and the practicability of the biopsy procedure.

Perform the following steps:

1. Connect the probe to the ultrasonic system and install the needle-guided bracket to the probe.
2. In B mode, press the **<Biopsy>** key to enter the Biopsy screen, a guide line displayed on the ultrasound image.
3. Select an appropriate needle-guided bracket and perform the guide line

calibration. Refer to “12.2.1 Calibrate the Biopsy Guide Line” for details.

4. Position the sampling target and make the target or lesion displayed on the guide line.

NOTE: DO NOT freeze the image when scanning or adjusting, otherwise the real-time biopsy process may fail to display.

5. Insert the needle through the needle guide hole and take a sample at the appropriate location.
6. After the biopsy procedure is completed, carefully remove the puncture needle from the animal.
7. Remove the needle-guided bracket from the probe and dispose of the disposable contaminated waste such as probe sheath as required by local regulations.
8. Press the **<Biopsy>** key again to exit the Biopsy screen.

12.2.3 Bracket Cleaning and Disinfection

To avoid cross-infection, please strictly follow the infection control policy formulated by the local hospital and clean and disinfect the needle-guided bracket after each biopsy.

- NOTE:**
- **Never disinfect the needle-guided bracket with a disinfectant containing chloride ion (Cl-) or fluoride ion (F-).**
 - **Always wear sterile gloves to avoid infection during cleaning and disinfection.**
 - **Low performance may result due to repeated disinfection, please change the needle-guided bracket as needed.**

Perform the following steps to clean and disinfect the needle-guided bracket:

1. After each use, remove the bracket from the probe. Use a small, soft brush to remove visible foreign matters from bracket surface and clean the metal lumen with the attached cleaning brush. Clean as soon as possible to avoid parts being dry and difficult to clean.
2. Immerse the bracket for at least five minutes in neutral pH low foam enzyme cleaner. When soaking, brush off the residual foreign matter. If visible foreign matters are difficult to remove, repeat the soaking procedure for another five minutes. Remove the bracket from the cleaning solution and wipe off all residues with a sterile cloth. Please follow the manufacturer's instructions for cleaner solution.
3. Immerse the bracket in 2% glutaraldehyde based solution for 10 hours at room temperature.
4. High-pressure steam sterilization. Autoclaving (134°C ± 4°C) for 20 minutes.

12.2.4 Bracket Storage and Transportation

The bracket is packed in non-sterile packaging. After sterilization, it should be properly stored in a sterile environment.

When using 2% glutaraldehyde based solution for disinfection and sterilization, the service life of the bracket is 2 years. When using High-pressure steam sterilization for disinfection and sterilization, the service life of the puncture frame is 5 years. Before discarding or returning to the manufacturer for maintenance, please disinfect and sterilize the bracket first.

Chapter 13 System Maintenance

To avoid the long-term exposure to dust and moisture which may result in poor performance and safety of the system, routine system maintenance should be performed by the user.



Warning

- **When cleaning the system, pay special attention not to let liquid enter any part of the system. Otherwise, electric shock may result. If liquid is accidentally into the system, stop cleaning the system immediately and shut down the system, contact Zoncare Customer Service Department or sales representative.**

NOTE:

- **Before cleaning procedure, shut down the system and unplug the power cord. Otherwise, electric shock may result.**
- **Maintenance shall be taken regularly to ensure the performance of the system, and ensure that the system is well grounded and meets the safety requirements.**
- **Except for the basic cleaning and maintenance described in this section, only personnel authorized by the manufacturer may perform other maintenance.**

13.1 External Cleaning

Perform the following steps:

1. Shut down and unplug the system.
2. Apply a few drops of 75% alcohol to moist a piece of lint-free cloth.
3. Gently wipe the display, touch screen, control panel, and other panel surfaces of the console with the lint-free cloth.

NOTE: Do not use cleaners or other cleaning fluids to clean the surface of the monitor.

4. Use a cotton swab to remove dirt from the control panel buttons to ensure that solid material does not fall into the console.
5. If blood or other infectious materials contact with the buttons or other parts of the system, wipe them with a 70% isopropyl alcohol solution.
6. Clean the air filter on the console regularly to ensure the cleanness and ventilation of the console.

13.1.1 Clean the Trackball

Perform the following steps:

1. Shut down and unplug the system.
2. Press the bulges on the clamping ring by two figures and turn the ring counterclockwise until it unlocked.

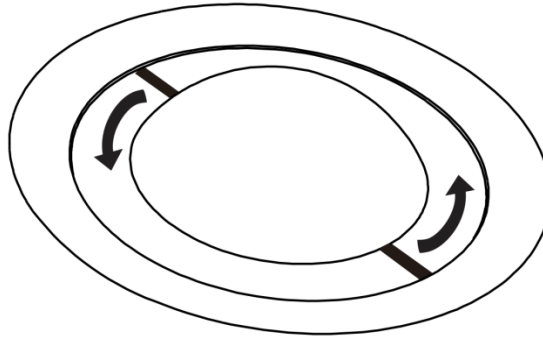


Figure 56 Unlock the Clamping Ring

3. Remove the clamping ring and take out the rotary ball.
4. Remove stains from the trackball and the ring with a soft, lint-free cloth to draw 75% alcohol.
5. Use a cotton swab to draw 75% alcohol to wipe the slot of the trackball.
6. After cleaning, put the trackball and clamping ring back and rotate it clockwise to fix it.

13.1.2 Clean the Probe Holder

Perform the following steps:

1. Move the probe holder towards the rear side of the system along the probe bracket and take out the probe holder.

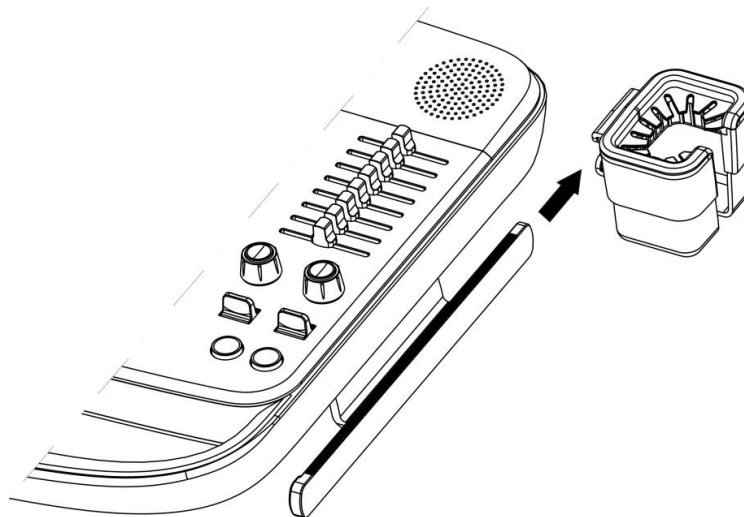


Figure 1 Take out the Probe Holder

2. Remove stains from the probe holder with a soft, lint-free cloth or brush to draw 75% alcohol.
 - If there are solid stains such as coupling gel, brush gently with a soft brush moistened with mild soapy water or detergent, and dry with a dry soft towel or air dry naturally.
3. After cleaning, put the probe holder back into the probe bracket.

13.1.3 Clean the Gel Warmer



Warning When cleaning the gel warmer, do not put the warmer under water, otherwise it will damage the electronic components inside the warmer.

Perform the following steps:

1. Remove the Gel warmer. Pull out the gel warmer power cord from the bottom of the control panel and move it along the probe bracket toward the back side of the system to remove the gel warmer.

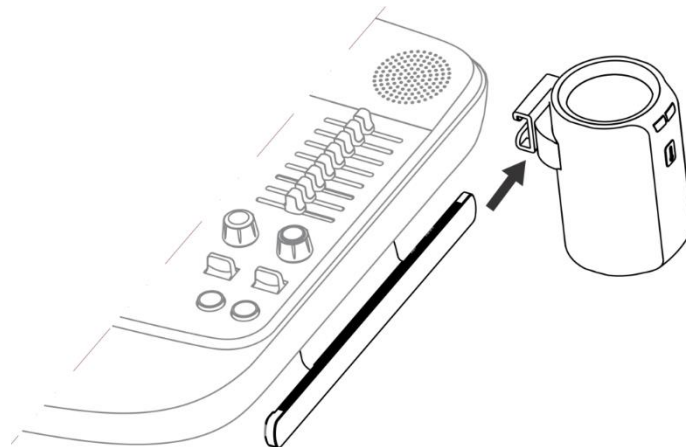


Figure 2 Remove the Gel Warmer

2. Clean the gel warmer.
 - 1) Press the two contact spring of the bottom cover with your fingers to remove the bottom cover.

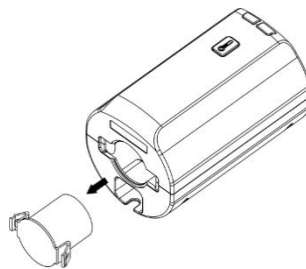


Figure 3 Remove the Bottom Cover

- 2) Remove stains from the warmer with a soft, lint-free cloth or brush to draw 75% alcohol.
- 3) If there is a large amount of coupling gel stuck in the bottom cover, clean the bottom cover with a brush dampened with mild soap or detergent and dry with a dry soft towel.

13.1.4 Clean the Printer

To clean the printer housing, please perform the following steps:

1. Before cleaning the printer, turn off the power and disconnect the power cord.
2. Use a clean and soft cloth to absorb an appropriate amount of isopropanol with

a concentration of 50~70v/v% or ethanol with a concentration of 76.9~81.4v/v% and wipe the printer surface.

3. Stubborn stains can be removed with a soft cloth such as a cleaning cloth slightly dipped in a mild detergent solution, and then cleaned with the above chemicals.
4. After cleaning, place the printer in a cool and ventilated environment to dry.

NOTE:

- Do not wipe the printer surface too hard, otherwise the printer surface may be damaged.
- Do not make the printer surface contact with rubber or vinyl products for a long time.

13.1.5 Clean the ECG equipment

To clean ECG cables and leads, please perform the following steps:

1. Unplug the ECG cable from the ECG lead port.
2. Wipe the surface of the cables and leads with a soft cloth slightly moistened (damp; not dripping) with 75% ethanol, and pay attention to avoid the metal parts.
3. Dry the cables and leads in a cool, ventilated environment.

13.2 Safety Check

To guarantee a high degree of operational reliability, regular inspection of the system by the maintenance and operating personnel is necessary for the following:

Table 46 Security Checklist

No.	Scope	Check item
1	Electrical safety	Inspect the cables for being broken or cracked.
		Check the grounding impedance.
		Check the leakage current.
		Check the animal leakage current.
		Check the animal auxiliary leakage current.
2	Mechanical Safety	Check the appearance.
		Check the control panel and keyboard.
		Check the knob and button.
		Check the casters.
		Check the ports.
3	Image Recording	Check display of each mode.
		Check parameter of each mode.
		Check image and report.

NOTE: Liquid or other substances seeping into the electronic components under the panel may result in intermittent failure of the control panel and

keyboard. Visually inspect for potential problems.

13.3 Troubleshooting

Table 47 Troubleshooting

No.	Failure	Measure
1	Power-on failure	● Check if the power cord is properly plugged into the power connector. ● Check if the circuit breaker is turned on. ● Check if the main power switch on the power supply panel is turned on.
2	No display on the monitor	● Check if the monitor is well connected. ● Check the brightness and contrast of the monitor.
3	The buzzer sounds and the buttons do not function.	Check if there is any button stuck on the control panel. If so, press the button to release the stuck button, and check if there is dirt under the stuck button and clean it promptly.
4	Abnormal image quality	● Check if the appropriate probe and mode are selected. ● Check if the relevant parameters are adjusted. For details, please refer to “Chapter 6 Optimizing the Image”. ● Check the related settings. For details, see “4.2 System Preset”.
5	Missing of application measurement item	● Check if the selected probe is applicable for current exam. ● Check if the application item is added.

When the above failures occur, and the corresponding measures still cannot solve, please contact the manufacturer or authorized personnel for further support. In the case of more difficult situations, please contact the manufacturer or authorized personnel.

13.4 Disposal

When the system, probe, needle-guide bracket and other accessories reach the end of their service period, they shall be disposed of according to the regulations on waste electrical and electronic equipment (WEEE) or local regulations.

Refer to manufacturer or supplier for information on disposal or recycle.

The manufacturer does not assume liability for any damage caused by unauthorized handling of the system without consulting.

NOTE: The definition of the WEEE label applies to EU member states only: The use of this symbol indicates that this system should not be treated as household waste. By ensuring that this system is disposed of correctly, you will help prevent bringing potential negative consequences to the environment and human health. For more detailed information with regard to returning and recycling this system, please consult the distributor from

whom you purchased the system.

For system products, this label may be attached to the main unit only.

13.5 After Sales Service

Service should only be provided by qualified technical personnel authorized by the manufacturer.

Contact the after-sales service department via following ways when you need technical support:

Manufacturer: Wuhan Zoncare Bio-medical Electronics co., Ltd

Address: #380, High-tech 2nd road, Eastlake high-tech district, Wuhan, Hubei, P. R. China

Zip code: 430206

Telephone: +86(27)87770581

Fax: +86(27)87770203

Website: <http://www.zoncare.com>

Appendix A. Technical Specifications

Safety Classification	Electrical shock	Class I (equipment with battery)	
	Degree of shock	Type BF Equipment	
	Operating mode	Continuous	
	EMC	CISPR 11 Class A	
	Installation and usage	Mobile equipment	
	Degree of protection, ingress	Console: IPX0 Probe: IPX7 Foot Switch: IPX4	
	Flammable mixtures	Not for use in presence of flammable anesthetic mixture with oxygen or nitrous oxide. Store the product in a dry and well-ventilated room. External grounding protection must be used to reduce possible external AC interference.	
Environment Requirements	/	Operating	Transport and storage
	Relative humidity	25%~85%	10%~95% (no condensation)
	Ambient temperature	5°C~+40°C	-20°C~+55°C
	Atmospheric pressure	800hPa~1060hPa	800hPa~1060hPa
Specification	Monitor	21.5" LCD	
	Touch Screen	13.3" touch screen	
	Dimension	528mm*607mm*1385mm	
	Weight	About 61kg	
Power Requirement	Power Supply	100-240V~	
	Power Supply Frequency	50Hz/60Hz	
	Input Power	100-240V~, 4-2.3A	
	Output Power	240VA	
	Circuit Breaker	250V~, 10A	
	Battery	14.4V/6500mAh	

Appendix B. EMC Statement



Warning

The use of unapproved accessories may diminish system performance.

Use of unapproved components, accessories, probes, and cables may result in increased emission or decreased immunity of system.

Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.

Use of accessories, probes and cables other than those specified or provided by the manufacturer of this the Ultrasound machine could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.

Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the Ultrasound machine, including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.

NOTE:

The system needs special precautions regarding EMC and needs to be installed and used according to the information provided in this section.

The EMISSIONS characteristics of this equipment make it suitable for use in industrial areas and hospitals (CISPR 11 class A). If it is used in a residential environment (for which CISPR 11 class B is normally required) this equipment might not offer adequate protection to radio-frequency communication services. The user might need to take mitigation measures, such as relocating or re-orienting the equipment.

Position system further from source of conducted RF noise to prevent conducted RF immunity.

This system is only used by professional medical staff. The equipment/system may cause radio interference or disrupt the operation of nearby equipment. Mitigation measures may be necessary, such as recalibrating the direction, resetting the device or shielding the appropriate site.

If the system is operated within the electromagnetic environment specified in following tables, the system will remain safe and provide the following basic performance:

- B-mode imaging function and resolution

Guidance and manufacturer's declaration – electromagnetic emission –for all EQUIPMENT AND SYSTEMS

1	Guidance and manufacturer's declaration – electromagnetic emission		
2	The ultrasound machine is intended for use in the electromagnetic environment specified below. The customer or the user of ultrasound machine should assure that it is used in such an environment.		
3	Emissions test	Compliance	Electromagnetic environment - guidance
4	RF emissions CISPR 11	Group 1	The ultrasound machine uses RF energy only for its internal function. There for, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
5	RF emissions CISPR 11	Class A	The ultrasound machine is suitable for use in all establishments other than domestic and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
6	Harmonic emissions IEC 61000-3-2	Class A	
7	Voltage fluctuations flicker emissions IEC 61000-3-3	Complies	

The approved annex which meets the electromagnetic standard:

Accessories for Ultrasound System may affect their radiation levels. The accessories listed in this section have been tested in accordance with international standards for use in Ultrasound System and have been verified to meet radiation standards. Please use only the attachments listed in this section.

The user should ensure the electromagnetic compatibility of the Ultrasound System when attaching accessories to Ultrasound System. Unless otherwise specified, use only EMC compliant equipment.

No.	Item	Cable length	Shield or not
1	Power cable	2 m	No
2	Probe cable	< 3 m	Yes
3	ECG cable	< 3 m	Yes
4	Printer cable	≤ 3 m	No
5	Printer USB cable	≤ 2.5 m	Yes
6	Foot Switch cable	≤ 3 m	Yes



Warning

- **This equipment is only used by professional medical staff. The equipment/system may cause radio interference or disrupt the operation of nearby equipment. Mitigation measures may be necessary, such as recalibrating the direction, resetting the device or shielding the appropriate site.**

Guidance and manufacturer's declaration – electromagnetic immunity – for all EQUIPMENT and SYSTEMS

Guidance and manufacturer's declaration – electromagnetic immunity			
The ultrasound machine is intended for use in the electromagnetic environment specified below. The customer or the user of the ultrasound machine should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Electrostatic discharge (ESD) IEC 61000-4-2	± 8 air kV contact ± 2 kV, ± 4 kV, ± 8 kV, ± 15 kV	± 8 kV contact ± 2 kV, ± 4 kV, ± 8 kV, ± 15 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30 %.
Electrostatic transient / burst IEC 61000-4-4	± 2 kV for power supply lines ± 1 kV for input/output lines	± 2 kV for power supply lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	± 1 kV differential mode ± 2 kV common mode	± 1 kV differential mode	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	0 % U_T ; 0,5 cycle g) At 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315° 0 % U_T ; 1 cycle and 70 % U_T ; 25/30 cycles Single phase: at 0° 0 % U_T ; 250/300 cycle	0 % U_T ; 0,5 cycle g) At 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315° 0 % U_T ; 1 cycle and 70 % U_T ; 25/30 cycles Single phase: at 0° 0 % U_T ; 250/300 cycle	Mains power quality should be that of a typical commercial or hospital environment.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	30 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

NOTE

1. U_T is the a. c. mains voltage prior to application of the test level.
2. When the interference signal is injected into the machine through the power line and generates interference on the transducer, the imaging system may have regular points or broken lines or line segments, but it will not be recognized as a physiological signal and does not affect the diagnosis.
3. During the discharge, the device has signal interference, and returns to the normal operation of the previous operating mode within 10 seconds without losing any user settings or stored data, and can continue to provide its expected functions and maintain basic performance, this phenomenon is acceptable.

Guidance and manufacturer's declaration – electromagnetic immunity – for EQUIPMENT and SYSTEM

Guidance and manufacturer's declaration – electromagnetic immunity			
The ultrasound machine is intended for use in the electromagnetic environment specified below. The customer or the user of the ultrasound machine should assure that it is used in such an environment.			
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance
Conducted RF IEC 61000-4-6 Radiated RF IEC 61000-4-3	3 Vrms 150 kHz to 80 MHz 6 V in ISM and amateur radio bands between 0,15 MHz and 80 MHz 10 V/m 80 MHz to 2.7 GHz 385MHz-5785MHz Test specifications for ENCLOSURE PORT IMMUNITY to RF wireless communication equipment (Refer to table 9 of EN 60601-1-2:2015)	3V 150 kHz to 80 MHz 6 V in ISM and amateur radio bands between 0,15 MHz and 80 MHz 10 V/m 80 MHz to 2.7 GHz 385MHz-5785MHz Test specifications for ENCLOSURE PORT IMMUNITY to RF wireless communication	Portable and mobile RF communications equipment should be used no closer to any part of the ultrasound machine, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance $d = \left[\frac{3.5}{V_1} \right] \sqrt{P}$ $d = \left[\frac{12}{V_2} \right] \sqrt{P}$ $d = \left[\frac{3.5}{E_1} \right] \sqrt{P} \quad 80 \text{ MHz to } 800 \text{ MHz}$ $d = \left[\frac{7}{E_1} \right] \sqrt{P} \quad 800 \text{ MHz to } 2.7 \text{ GHz}$ where p is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, a should be less than the

		equipment (Refer to table 9 of EN 60601-1-2:2015)	compliance level in each frequency range. Interference may occur in the vicinity of equipment marked with the following symbol: 
NOTE 1 At 80 MHz and 800 MHz, the higher frequency range applies. NOTE 2 These guidelines may not apply in all situations. Electromagnetic is affected by absorption and reflection from structures, objects and people.			
a The ISM (industrial, scientific and medical) bands between 150 kHz and 80 MHz are 6,765 MHz to 6,795 MHz; 13,553 MHz to 13,567 MHz; 26,957 MHz to 27,283 MHz; and 40,66 MHz to 40,70 MHz. The amateur radio bands between 0,15 MHz and 80 MHz are 1,8 MHz to 2,0 MHz, 3,5 MHz to 4,0 MHz, 5,3 MHz to 5,4 MHz, 7 MHz to 7,3 MHz, 10,1 MHz to 10,15 MHz, 14 MHz to 14,2 MHz, 18,07 MHz to 18,17 MHz, 21,0 MHz to 21,4 MHz, 24,89 MHz to 24,99 MHz, 28,0 MHz to 29,7 MHz and 50,0 MHz to 54,0 MHz. b Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the ultrasound machine is used exceeds the applicable RF compliance level above, the ultrasound machine should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the ultrasound machine. c Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3V/m.			

**Recommended separation distances between portable and mobile
RF communications equipment and the EQUIPMENT or
SYSTEM -
for EQUIPMENT and SYSTEMS**

Recommended separation distances between portable and mobile RF communications equipment and the ultrasound machine				
The ultrasound machine is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the ultrasound machine can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the ultrasound machine as recommended below, according to the maximum output power of the communications equipment				
Rated maximum output of transmitter W	Separation distance according to frequency of transmitter (m)			
	150 kHz to 80 MHz outside ISM and amateur radio bands $d = [\frac{3.5}{V_1}] \sqrt{P}$	150 kHz to 80 MHz in ISM and amateur radio bands $d = [\frac{12}{V_2}] \sqrt{P}$	80 MHz to 800 MHz $d = [\frac{3.5}{E_1}] \sqrt{P}$	800 MHz to 2.7 GHz $d = [\frac{7}{E_1}] \sqrt{P}$
0.01	0.12	0.20	0.035	0.07
0.1	0.38	0.63	0.11	0.22
1	1.2	2.00	0.35	0.70
10	3.8	6.32	1.10	2.21
100	12	20.00	35	70
For transmitters rated at a maximum output power not listed above the recommended separation distance d in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.				
NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.				
NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.				

Appendix C. Toxic and Hazardous Substances or Elements

Parts	Toxic and harmful substances or elements					
	Plumbum (Pb)	Mercury (Hg)	Cadmium (Cd)	Chromium 6 (Cr6+)	PBB	PBDE
Plastic case	○	○	○	○	○	○
Metal bracket	○	○	×	×	○	○
Keyboard silicone	○	○	○	○	○	○
Trackball	×	○	○	○	○	○
Cables	×	○	○	○	○	○
PCBA	×	○	○	○	○	○
Hard disk	○	○	○	○	○	○
○: Means that the content of the toxic and harmful substance in all homogeneous materials of the part is below the limit specified in local standard. ×: It means that the content of the toxic and harmful substance in at least one homogeneous material of the part exceeds the limit requirement specified in the local standard. For products sold since the date of sale, this table shows that products in our supply chain may contain these substances. NOTE: all listed components may or may not be included in the products sold.						

No. 1821064500



Wuhan Zoncare Bio-medical Electronics Co., Ltd.

Address: #380, High-tech 2nd road, Eastlake high-tech district, Wuhan, Hubei, P. R. China

Tel: +86(27)87770581

Tel/Fax: +86(27)87770203 Post Code: 430206

<http://www.zoncare.com> Email: info@zoncare.com